

Mobile medical systems for equitable healthcare

Justin Chan¹, Mayank Goel¹, Shyamnath Gollakota²✉ & Rajalakshmi Nandakumar³

Abstract

Major barriers to accessible healthcare include the high cost of medical devices and limited healthcare facilities. Mobile computing technologies, such as smartphones and smart watches, include high-quality hardware, such as microphones, speakers and cameras, which can be leveraged for the design of low-cost mobile medical systems intended to be remotely applied to monitor health and disease. In this Review, we discuss low-cost and accessible hardware – in particular, mobile phones – that can be used in mobile medical systems to aid in medical diagnostics and monitoring. Specifically, we outline acoustic-based systems, vision-based systems and sensor fusion systems that allow different levels of health and disease assessment, relying on the speakers, microphones and sensors of smart mobile devices. We highlight the challenges related to the deployment of mobile medical systems in the clinical continuum, including scaling, generalizability, bias, trust and privacy. Finally, we examine clinical integration and regulatory considerations with regard to mobile medical devices as well as future applications.

Sections

Introduction

Acoustic-based systems

Vision-based systems

Sensor fusion systems

Custom low-cost sensing systems

Real-world challenges

Trust in mobile health systems

Regulatory considerations

Clinical integration and automated interventions

Outlook

¹School of Computer Science, Carnegie Mellon University, Pittsburgh, PA, USA. ²Paul G. Allen School of Computer Science, University of Washington, Seattle, WA, USA. ³Department of Information Science, Cornell Tech, New York, NY, USA. ✉e-mail: gshyam@cs.washington.edu

Key points

- Mobile medical systems leverage smart devices and their sensing capabilities for the remote detection of health conditions.
- Acoustics-based systems rely on microphones and speakers to monitor vital signs in a contactless manner and to passively sense audible biomarkers to detect medical conditions.
- Vision-based systems combine cameras and actuators in smart devices with computer vision algorithms to track physiological signals, diagnose medical conditions and analyse biofluids.
- Sensor fusion systems combine passively measured sensor data, digital activity traces and questionnaire responses to assess digital biomarkers associated with physical, mental and behavioural health.
- The scaling and adoption of mobile medical systems require generalizability to diverse hardware designs, adaptation to real-world environments, assurance of patient privacy and mitigation of clinical bias.

Introduction

Medical resources and devices are not equitably accessible around the globe, partly owing to the high costs of medical devices and limited healthcare facilities^{1–3}. For example, hearing care⁴ in low-resource and rural regions often relies on outdated diagnostic hardware, donated by non-profit foundations, such as [Hear the World](#), and patients often have to travel a long distance for hearing screenings⁵. Similarly, blood-clot tests are essential for individuals who need to take blood thinners but these tests are expensive or have to be conducted in laboratories. As a result, such patients might remain in an acceptable blood-clotting range for only 40% of the time owing to less frequent testing^{6–8}. In addition, rare diseases, such as speech impediments, might affect only a small population, and thus financial incentives to invest in research and development on rare conditions might be limited.

Mobile computing technologies, including smartphones and earphones, can incorporate high-quality microphones and speakers, and cost US\$40–50 second-hand, which is substantially lower than the cost of a typical medical device. Such mobile devices can be leveraged for the design of medical systems for large-scale diagnostics and monitoring through the co-design of sensor hardware and software using machine learning, wireless sensing and signal-processing tools. For example, onboard sensors, such as acoustic sensors in a smartphone, enable the detection of breathing irregularities associated with sleep apnoea⁹ and opioid-induced respiratory depression¹⁰. Similarly, passive acoustic monitoring systems can detect lung disorders through cough sounds¹¹, and digital phenotyping systems^{12–14} can assess physical activity or irregular speech patterns by combining data from different sensors. In addition, low-cost tools can be attached to mobile devices; for example, a paper cone to detect middle-ear fluid¹⁵ or a 3D-printed plastic holder to collect a small blood sample for blood clot testing¹⁶, a whistle-like device for spirometry lung-function testing¹⁷ or a smartphone clip that guides the user to press their finger against the camera for blood-pressure testing¹⁸.

In addition to the standard sensors included in mobile devices, such as red–green–blue (RGB) cameras, microphones, speakers and

inertial measurement units (IMUs), light detection and ranging (LiDAR) sensors, depth cameras, high-frequency ultrasound, slow-motion cameras, projectors and ultrawideband radios might be exploited in the engineering of mobile medical systems. Moreover, smartphone processors including graphics processing units, such as Apple's neural engine, which are specialized cores functioning as a neural processing unit, allow on-device machine learning applications and can be explored for real-time speech translation or privacy-preserving, passive sensing of acoustic biomarkers to track neurological processes.

Smart devices, such as smart speakers, smart watches, wireless earbuds and smart eyewear, can serve as sensing platforms in mobile health sensing (Box 1). For example, active sonar and beamforming technology in smart speakers allows the measurement of the respiratory rates of infants using white noise¹⁹ and heart rhythm assessment in adults²⁰. In-ear devices can be applied for ear health assessment, for example, by measuring eardrum mobility to detect middle-ear fluid¹⁵ and disorders²¹, as well as to screen for hearing loss by measuring otoacoustic emissions^{22–24}. Furthermore, wearable cameras can be applied to identify medication errors²⁵, and smart eyewear can be used in augmented-reality assisted surgery^{26–28}.

In this Review, we discuss advances, challenges and future directions in the field of mobile health systems (Fig. 1). We focus on technologies that leverage consumer smart devices (smartphones, smartwatches, smart speakers, smart glasses, smart eyewear and earbuds) as platforms for sensing and health assessments (Table 1). Thanks to the accessibility, economies of scale and sensing capabilities of these devices, they could support global access to high-quality healthcare (Box 2). We categorize mobile medical systems according to their primary sensing modality into: acoustic-based systems, which have both active and passive sensing approaches; vision-based systems, which leverage RGB cameras for motion tracking, colour analysis and scene understanding; and sensor fusion systems, which combine passive sensor data (for example, IMUs, radio signal strength and light sensors), digital activity traces and user questionnaires to measure digital biomarkers for individual-scale and population-scale health sensing, such as in digital contact-tracing systems for epidemiological tracking. Finally, we highlight mobile systems that use custom but low-cost sensing systems for healthcare monitoring.

Acoustic-based systems

Acoustic-based systems, comprising active sonar and passive sensing systems, exploit built-in speakers and microphones. Active sonar systems emit custom sound from the speaker, while recording from the microphone, thereby enabling contactless monitoring by measuring human motion, such as breathing and heartbeats, based on acoustic reflections. Such systems can also be used for point-of-care testing of ear-related health conditions. Passive sensing systems rely solely on the microphone to record acoustic biomarkers, and can be used to detect cardiac arrest events from a smart speaker²⁹, respiratory function over a telephone line¹⁷ and cough sounds using a neck-worn phone¹¹.

Active sonar systems

Contactless monitoring systems (Fig. 2) leverage active sonar signals to track human motion by transmitting inaudible acoustic signals in the 18–22-kHz frequency band. Audible noise and interference, including human speech <18 kHz, can be filtered out, which enables privacy preservation¹⁰. These systems allow at-home monitoring of medical conditions. Individuals can self-administer the test and share the results virtually with their physician, thus improving access to healthcare.

In addition, individuals in home isolation or quarantine settings can be monitored, reducing the burden of regularly disinfecting contact-based wearable devices.

ApneaApp⁹ is a contactless monitoring system that uses a smartphone to track fine-grained breathing and motion patterns of the chest and abdomen to detect sleep apnoea and hypopnoea events by continuously transmitting inaudible frequency-modulated continuous-wave (FMCW) signals and analysing the reflections that bounce off the chest of an individual (Fig. 2a–d). ApneaApp has been evaluated in a clinical study at a sleep laboratory against gold-standard polysomnography on apneic patients, demonstrating a high degree of accuracy in identifying sleep apnoea events. The active sonar principle in smartphones can also be applied for opioid-overdose detection¹⁰ by identifying respiratory depression, apnoeas and large movements correlated with opioid toxicity. In a supervised injection facility and an operating room environment with simulated opioid-overdose events, this overdose detection system could accurately identify overdose events. SpiroSonic³⁰ exploits active sonar to measure chest-wall motion, which is transformed into indices of lung function, whereas PTEase³¹ measures reflections from an individual's airway using a mouthpiece to measure the cross-sectional area of each airway segment.

Smart speakers that support an array of six to seven microphones enable fine motion tracking through complex acoustic signal-processing algorithms (Fig. 2e–g). By extracting submillimetre body displacements caused by the chest wall, smart speakers can filter out larger breathing motions and ambient noise to identify individual heartbeats and compute the heart rate and R–R intervals (interbeat interval, measured between successive R-peaks in ECG signal) for healthy users and users with cardiac abnormalities²⁰. BreathJunior¹⁹ can monitor subtle breathing motions of infants in the neonatal intensive care unit (NICU) using white-noise signals. A contactless approach is particularly desirable for infants, given that wires and contact sensors can cause rashes, burns and, in rare cases, death from strangulation^{32,33}.

Earable systems are designed to detect medical conditions and measure physiological signals from the ear (Fig. 3). Active sonar earable systems can detect middle-ear fluid by sending a soft acoustic chirp at 1.8–4.4 kHz through a paper funnel into the ear canal, measuring reflections to assess eardrum mobility¹⁵ (Fig. 3a–c). An ear without fluid allows most sound to pass through the eardrum, whereas fluid buildup causes the eardrum to stiffen and reflect more sound energy. This platform shows comparable performance to specialist tools, such as tympanometry and pneumatic otoscopy, and can be performed by non-specialists. EarHealth³⁴ can assess ear disorders using a modified wired earphone with an in-ear-facing microphone and speaker to probe the ear. The system can detect ears that are normal, filled with fluid, blocked with earwax or that contain a ruptured eardrum. Wireless earbuds²³ and smartphone earbuds²⁴ allow low-cost newborn hearing screening (Fig. 3d–f) by probing the cochlea with sounds that cause cochlea hair cells to vibrate. A microphone detects the sounds produced from the vibrations to assess hearing status. This system achieves clinical accuracies comparable to the gold-standard [hearing screening devices](#) cleared by the US Food and Drug Administration (FDA), which are orders of magnitude more expensive. An open-source, portable, smartphone-based attachment²¹ can be applied to measure middle-ear function and help to diagnose middle-ear disorders. The attachment probe forms a seal with the ear canal, safely varies air pressure and generates a tympanogram to quantify eardrum mobility. APG³⁵ uses active noise-cancelling headphones to send ultrasound signals into the ear canal to monitor cardiac events. Blood-vessel deformation

Box 1 | Translational considerations

Mobile medical systems are typically based on a proof-of-concept prototype that relies on built-in sensors of a smart device and/or custom low-cost attachments^{15–18} to augment the device's sensing capabilities. Translating a prototype into a deployable system requires consideration from multiple stakeholders.

Reimbursement considerations

Medical expenses can be reimbursed by insurance companies. In the USA, mobile health systems can be designed to conform to insurance codes, such as the current procedural terminology (CPT) codes used by Medicare and Medicaid. For example, smartphone-based middle-ear-fluid detection by acoustics¹⁵ is reimbursable under the Medicare and Medicaid CPT code 92567. Mobile health companies, such as Eko Health, have been approved for a new CPT code to cover the [SENSORA digital stethoscope](#) that detects heart diseases using artificial intelligence algorithms. Integration with an insurance system might thus promote adoption.

Human factors design

Users should be considered in the design of a mobile medical system. If the intended user is a medical professional, hardware design and software user interfaces should resemble to familiar medical devices to streamline adoption and minimize usability concerns. If the intended user is a layperson, the device should present an easily interpretable medical result with actionable suggestions.




Balancing true and false positives

Mobile medical systems are often designed to produce a binary result, indicating the presence or absence of a disease or medical event. Screening or early detection tests intended for broad population testing typically prioritize achieving a high true-positive rate, even if this might result in an increased false-positive rate. This approach is justified only if the medical consequences of a false-positive result are minor, given that a positive result is typically followed up by more accurate diagnostic tests for confirmation. Diagnostic systems require a high true-positive rate and a low false-positive rate to yield an accurate result without generating unnecessary false alarm.

leads to minute changes to the ear-canal volume, which can be tracked by this system using ultrasound reflections to measure heart rate and heart-rate variability.

Passive sensing systems

Audible biomarkers in non-speech and speech sounds can be detected using ambient sensing systems that leverage voice assistants on smartphones or smart speakers to passively listen for medical events. These systems can track medical conditions long-term and thus have the potential to identify medical conditions that are difficult to detect in isolated clinic visits. However, such passive sensing systems require high levels of specificity to avoid false-positive events, must be generalizable to multiple environments with varying ambient noise profiles, and must address privacy concerns in relation to always-on microphones by operating locally without sending data to the cloud.

	Acoustic-based systems	Vision-based systems	Sensor fusion systems
Smartphone 	Physiological signals Breathing, heartbeats, eardrum mobility, body sounds (coughing, eating events, motions), heart sounds, cochlea response Health conditions Sleep apnoea, opioid-induced respiratory depression, middle-ear fluid, lung function, respiratory conditions (e.g. asthma, cystic fibrosis, COPD, COVID-19, flu)	Physiological signals Breathing, heart rate, PPG, haemoglobin, blood-oxygen saturation, seismocardiograph, blood pressure, capillary refill time, intra-ocular pressure, blood glucose, microsleep events Health conditions Concussion, jaundice, anaemia, diabetic retinopathy, hypoxaemia, blood-clotting times, proteinuria	Health conditions Depression, anxiety, schizophrenia symptoms, mood, fatigue, sleep quality, stress
Smart speaker 	Physiological signals Infant breathing, heartbeats, agonal breathing (precursor to cardiac arrest), speech patterns (e.g. Parkinson's disease)		
Earables 	Physiological signals Heart rate, heart sounds, teeth movement Health conditions Hearing loss		Health conditions Bruxism, sleep stages, epileptic seizures, blood pressure
Smart watch 			Health conditions ADHD

● Microphone
● Camera
● Speaker
● LiDAR

Fig. 1 | Mobile medical systems. Smart devices contain an array of sensors, including acoustic and vision sensors, which can be used for measuring physiological signals and health conditions. Passive sensor data can also be

fused to obtain a readout. ADHD, attention-deficit hyperactivity disorder; COPD, chronic obstructive pulmonary disease; LiDAR, light detection and ranging.

Detecting non-speech audible biomarkers. Non-speech body sounds have been proposed as privacy-preserving biomarkers for health conditions. For example, smart speakers can detect agonal breathing²⁹, an audible biomarker that occurs in more than half of cardiac arrests and when an individual experiences low oxygen levels^{36,37}. Such smart speakers can connect individuals that experience a cardiac arrest to emergency medical services in a timely manner. This system has been trained with 911 audio recordings of cardiac arrests to classify agonal breathing instances in real time in a bedroom setting. PDVocal³⁸ enables passive detection of Parkinson's disease by identifying breathing and sniffing sounds that indicate declining lung health and early signs of Parkinson's disease. BodyBeats³⁹ relies on a wearable piezoelectric microphone embedded in a neckpiece that is in contact with the user's skin to capture body sounds, such as eating, drinking, breathing, laughing and coughing.

Coughing, in particular, can serve as an early detection marker for a variety of respiratory conditions, such as asthma⁴⁰, cystic fibrosis⁴¹ and chronic obstructive pulmonary disease (COPD)⁴². Privacy-preserving cough detection systems¹¹ analyse audio from a mobile phone placed in a user's shirt pocket or worn around the neck. To preserve patient privacy, the system applies principal component analysis to spectrograms

for audio classification. For example, crowdsourced, passively sensed audio of coughing, breathing and speech can be used to detect COVID-19 (refs. 43–46) track disease progression over time^{47,48} and distinguish the coughing of multiple people⁴⁹. FluSense⁵⁰ captures coughs and speech using a microphone array, combined with thermal camera videos, to predict influenza caseloads in hospital waiting areas.

Tracking speech patterns. Speech recordings can be analysed to identify patterns associated with disease. For example, Parkinson's disease affects the vocal tract, making it challenging to speak. Therefore, the progression of Parkinson's disease can be monitored by analysing speech patterns^{51,52}. StressSense⁵³ passively senses stress from human voices in conversations recorded in indoor and outdoor environments, and compares predictions with skin-conductance data from a wrist band. EmotionSense⁵⁴ uses acoustic features to categorize speech into broad emotional categories, such as happy, sad, scared, angry and neutral.

Physiological sensing using earables. Passive acoustic sensing systems can also be applied in earable systems that use in-ear microphone earbuds to measure physiological signals, taking advantage of the

occlusion effect. This effect occurs when the ear canal is blocked, such as when wearing earbuds, causing users to perceive an amplification of low-frequency bone-conduction sounds that occur during human motion. Using an in-ear microphone, OESense⁵⁵ can sense motion to recognize step counting, activity and hand-to-face gestures, and hEART⁵⁶ measures heart rate during user motion, outperforming in-ear photoplethysmography (PPG). A custom in-ear microphone in a wired earbud design can detect low-frequency infrasonic vibrations (<20 Hz) caused by heart sounds⁵⁷. This system can thus measure heart rate and interbeat interval, and differentiate between atrial fibrillation and sinus rhythm with an accuracy comparable to ground-truth electrocardiogram (ECG) measurements.

The raw audio stream recorded by commercial in-ear microphones is typically not accessible. Therefore, custom hardware design is required, or the microphone must be wired out to capture the audio signal. Alternatively, the in-ear speaker of earbuds can be repurposed as an input transducer to measure signals from the ear. For example, EarSense⁵⁸ uses the in-ear speaker to record teeth gestures, such as tapping and sliding, from different regions of the mouth. This system has been evaluated with interfering user motions caused by walking, nodding, cooking and cycling. Asclepius⁵⁹ converts earphones into a stethoscope, using the in-ear speaker to capture minute heartbeats from inside the ear and to reconstruct phonocardiogram signals for remote cardiac auscultation.

Point-of-care testing. Point-of-care tests can be administered on a smartphone to detect audible biomarkers. For example, SpiroSmart⁶⁰

measures lung function on a smartphone by having the user breathe in and forcefully exhale into the microphone. By analysing audio features in the time and frequency domains, the flow rate can be computed, with an accuracy comparable to that of a clinical spirometer. SpiroCall¹⁷ extends this capability to low-end mobile phones, such as feature phones that lack the processing power to locally process acoustic data. In this system, acoustic data is sent over a standard voice telephony channel, which degrades the audio quality, to an external server that provides algorithms to estimate the flow rate. In addition, a 3D-printed whistle accessory ensures an ideal testing setup for users with lower flow rates or who have difficulty performing the test.

Vision-based systems

Cameras are prevalent in smartphones, with many featuring front- and rear-facing cameras, which can capture high-resolution images and videos. Some smartphone models further contain a LiDAR scanner with a near-infrared camera, typically used for facial identification, and slow-motion cameras with high frame rates of 960 frames per second. Moreover, extended-reality devices for virtual and augmented reality typically contain multiple RGB and depth cameras for scene understanding as well as eye-tracking cameras. Vision-based systems can also be adapted for medical testing. For example, motion-tracking systems can report on physiological signals by tracking subtle body movements in video over time using computer vision algorithms (Fig. 4a). Colour-analysis systems can detect colour changes on an individual’s body related to vital signs or disease

Table 1 | Acoustic- and vision-based sensing technologies

Sensor	Sensing technique	Clinical applications	Deployed systems	Opportunities and limitations
Microphone and speaker	Active sonar	Vital signs: breathing ^{23,24} ; heartbeats ^{20,35} Medical events: apnoea ⁹ ; opioid-induced respiratory depression ¹⁰ Ear disorders: middle-ear fluid ^{15,21} ; newborn hearing loss ^{22–24}	BreatheEasy, SleepScore app	Opportunities: continuous monitoring by always-on, low-power sensors; contactless sensing; can be integrated into most smart devices Limitations: sensitivity to ambient background noise; privacy concerns; dataset collection and curation; potential for false positives; requires sensor calibration across different devices
	Passive acoustic sensing	Non-speech biomarkers: agonal breathing to detect cardiac arrest ^{17,60} ; breathing and sniffing sounds to detect Parkinson’s disease ³⁸ ; coughing to detect respiratory conditions (such as asthma, cystic fibrosis, COPD, COVID-19, flu) ^{1,43–50} . Speech patterns: Parkinson’s disease ^{52,222} ; stress sensing ⁵³ ; emotion sensing ⁵⁴ Physiological signals: heart rate; heart rate variability; interbeat interval ^{56,57} ; phonocardiogram ⁵⁹ ; teeth movement ^{58,103} ; step counting ⁵⁵ Point-of-care testing: measuring lung function ^{17,60}	Digital Wellbeing app for Pixel phones	
	Time-of-flight ranging	Digital contact tracing	TraceTogether ¹⁰⁹ Exposure notifications	
Camera	Motion tracking	Vital signs: breathing and heart rate ^{61–68} , Eye testing: pupillometry ^{70–72} ; intra-ocular pressure ⁷³ ; microsleep events ⁷⁴ Biofluid sensing: blood clotting ^{16,77} ; protein concentration in urine ⁷⁶	Google Fit for Pixel phones (breathing), Minuteful Kidney	Opportunities: contactless sensing; captures spatial, temporal and colour dimensions Limitations: privacy concerns; sensitivity to ambient lighting conditions; might require high power, thereby reducing battery life if used for continuous monitoring; requires sensor calibration across different devices; accuracy may differ across skin tones for certain tests
	Colour analysis	Blood testing: haemoglobin levels ^{78–80} ; oxygen saturation ^{81,82} ; blood pressure ^{18,83,84} Skin testing: jaundice ^{85,86} ; anaemia ⁸⁷ ; capillary refill time ⁹⁰ Eye testing: diabetic retinopathy; diabetic macular oedema and poor blood glucose control ⁸⁹ ; jaundice ⁸⁷	Google Fit for Pixel phones (heart rate)	
	Scene understanding	Medication errors ²⁵ Medical student training ⁹¹ Surgical tool tracking ^{92–95}	—	

COPD, chronic obstructive pulmonary disease.

Box 2 | Low-resource considerations

Medical devices are often designed for well resourced clinical environments. By contrast, mobile medical systems can provide solutions for regions that lack clinical resources and infrastructure. However, this requires several key design considerations.

Unreliable internet connectivity

Network connectivity issues can prevent mobile devices from connecting to the internet, posing challenges for systems that rely on the sending and receiving of medical data from machine learning models to and from the cloud. Alternatively, large machine learning models can be miniaturized to allow on-device inference using techniques such as pruning¹⁸³, quantization¹⁸⁴ and distillation¹⁸⁵.

Power outages

Medical devices typically require a wall outlet for power and are not designed to work in the event of electrical failures. Electrical failures can also result in the loss of lighting, which may be necessary for mobile systems that rely on cameras and vision-based techniques. Therefore, such systems need to work under a range of lighting conditions and with only the aid of a smartphone flash.

Noisy environments

Noisy environments can pose a challenge to mobile medical systems that leverage acoustics. Noise detection and cancellation algorithms can help to mitigate the effect of noise. Furthermore, ultrasonic sensing at >18kHz can be applied for the sensing of breathing, heartbeats and human motion^{8,10,19,20}.

Shortage of trained professionals

Mobile medical systems must be designed to be usable by individuals with limited expertise, and they should output actionable results that are easily interpretable.

Optimizing for limited sensing and computation capability

If smartphones with high-fidelity sensors are limited, mobile systems can be designed for low-cost feature phones, for example, to measure lung function using spirometry over a standard telephony voice channel¹⁷ or to perform audio-based privacy-preserving cough detection¹¹.

(Fig. 4b). Scene-understanding systems use wearable camera systems in extended-reality devices, applying real-time computer vision algorithms to automatically streamline manual tasks, for example, in the operating room.

Motion-tracking systems

Tracking vital signs. Computer vision algorithms can track subtle changes in videos of the face captured by cameras, detecting chest movements corresponding to individual breaths and identifying head motions caused by blood flow, which can be mapped to individual heartbeats^{61–68}. JoulesEye⁶⁹ uses a smartphone thermal camera system to measure respiration during high-intensity exercise and to estimate calorie burn. This system has been validated against ground-truth ECG, PPG sensors and respiration belts. Such capabilities are commercially

available and can [capture breathing rate by tracking chest movements from the front-facing camera](#).

Eye testing. PupilScreen⁷⁰ assesses the pupillary light reflex through a head-mounted smartphone display. The smartphone's flash stimulates the user's eye while recording changes to their pupil size over time to determine whether the pupil's response indicates traumatic brain injuries, such as concussions. The same test can also be performed without a head-mounted attachment⁷¹ by combining images from a front-facing RGB camera and a near-infrared camera, typically used for facial recognition. Alternatively⁷², just the RGB camera and a long-pass filter eye attachment can be applied to perform pupillometry across individuals with different levels of melanin in the irises. Intra-ocular pressure can also be measured with a smartphone-based attachment that emulates a fixed-force tonometry test⁷³. CarSafe⁷⁴ measures eye events, such as microsleep events and blinking rates, which can indicate drowsy driving, using the front-facing camera. Similarly, distracted driving phone usage⁷⁵ can be detected by distinguishing drivers and passengers using their phones and computer vision techniques.

Biofluid sensing. The smartphone camera can be combined with built-in actuators for biofluid sensing, without requiring additional electronic attachments. For example, a vibration motor and camera on a smartphone can be applied to measure blood-clotting time, requiring only 10 µl of blood¹⁶. The blood sample is deposited into a rubber cup that contains a copper particle and that is attached to a plastic cup holder coupled to the phone. The vibration motor causes the sample to vibrate and the copper particle to move around. Computer vision algorithms track when particle motion comes to a standstill, which occurs when the blood coagulates and thickens. CapCam⁷⁶ can measure the surface tension of urine to detect elevated protein concentration levels, indicating a high risk for proteinuria; here, the smartphone is placed over a cup of urine to capture capillary waves caused by the vibration motor. The wavelength between the crests and troughs of the ripples is then used to measure liquid surface tension. The LiDAR sensor has been explored to determine fluid properties of small liquid samples⁷⁷. When the LiDAR beam is projected onto a sample of liquid, a characteristic laser speckle pattern forms owing to light scattering from suspended particles, such as red blood cells and platelets in blood or fat and protein globules in milk. By characterizing the Brownian motion in the liquid, the viscosity states associated with coagulated and uncoagulated drops of blood can be distinguished.


Colour-analysis systems

Measuring vital signs. Colour-analysis systems can track vital signs from videos captured by a smartphone's rear-facing camera. In HemaApp^{78–80}, users place their finger over the back camera with the flash on and the system analyses subtle colour changes to estimate an individual's haemoglobin concentration level to screen for anaemia, with performance similar to FDA-approved haemoglobin measurement devices. The Google Pixel phone uses this technique to [measure colour changes caused by blood moving through the fingertip to compute heart rate](#). Blood-oxygen saturation levels can be measured to detect hypoxaemia, with similar performance to pulse-oximeter readings^{81,82}. Seismo⁸³ uses the smartphone's accelerometer to capture heart-valve vibrations and measure seismocardiography data by placing the phone on the user's chest. This is combined with PPG breathing data from the camera to compute pulse transit time and diastolic blood pressure.

However, Seismo requires initial calibration using a blood-pressure cuff for each user. By contrast, for BPClip⁸⁴, this calibration step can be bypassed with the aid of a low-cost mechanical smartphone attachment

that measures blood pressure using the oscillometry principle: the user places their finger onto a spring-loaded mechanism attached to the smartphone camera and gradually applies pressure, resulting in

Contactless detection of sleep apnoea and opioid overdose on a smartphone

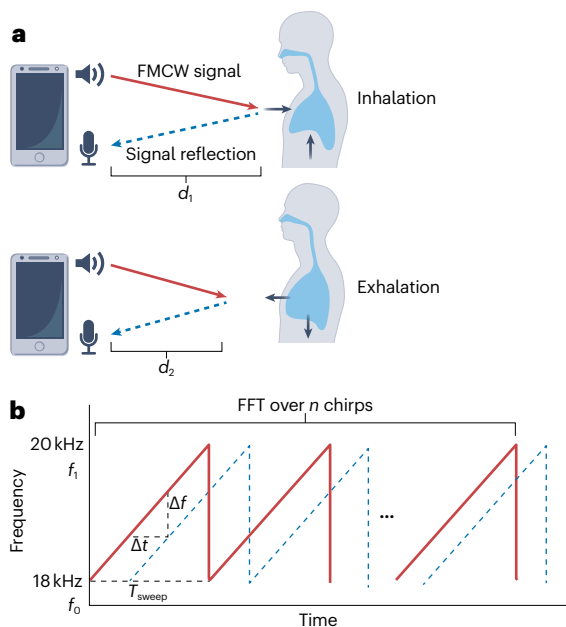

Contactless monitoring of heart rhythm by smart speakers


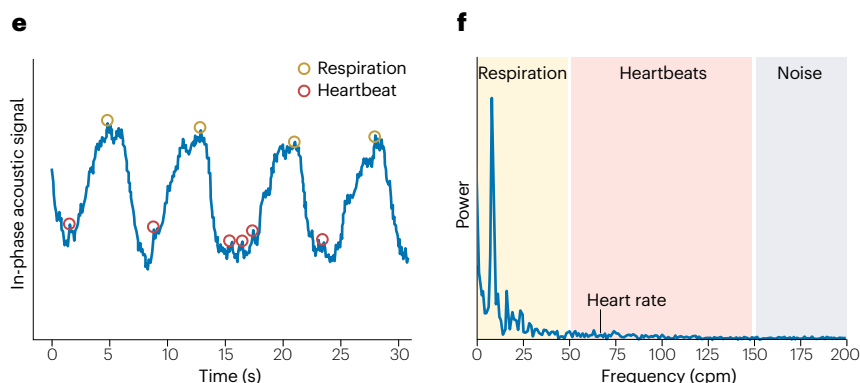


Fig. 2 | Contactless monitoring of vital signs using active sonar.

a–d, Contactless detection of sleep apnoea⁹ and opioid overdose¹⁰ on smartphones. **a**, Breathing can be measured in a contactless manner using active sonar on a smartphone. The speaker transmits an inaudible, frequency-modulated continuous-wave radar (FMCW) signal, which is reflected by the chest and recorded using the microphone. Changes in the breathing signal can be related to sleep apnoea and opioid overdose. d_1 and d_2 denote the distance between the smartphone and the chest during inhalation and exhalation respectively. **b**, The transmitter continuously transmits signals, in which the frequency increases linearly with time between frequencies f_0 and f_1 over a duration T_{sweep} . Reflections arriving with a time delay Δt create a frequency shift Δf . To extract the minute frequency shifts created by breathing motion, the receiver performs a fast Fourier transformation (FFT) over an integer number of chirps n . **c**, Over the course of multiple breathing cycles, reflections from the chest arrive at time delays Δt_i and Δt_e , when breathing in and out. These changes translate to distinct frequency shifts Δf_i and Δf_e , which can be estimated by taking an FFT over the chirps.

d, The breathing signal is located in a frequency bin corresponding to the individual's distance from the smartphone. Environmental motion occurs at a different distance and would thus appear in a different frequency bin, which can be filtered out. t_k , time point k ; t_{k+x} , time point $k+x$; t_n , time point n . **e–g**, Smart speakers can be applied to monitor heart rhythms in a contactless manner²⁰. **e**, When using active sonar to measure heartbeats, the breathing motion is strong, but the heartbeats are weak and difficult to observe. **f**, In the frequency domain, harmonics produced from the breathing signal spread out into the bins corresponding to heart-rate range and therefore cannot easily be filtered out. **g**, Beamforming and signal-processing algorithms running on a smart speaker system can be used to extract individual heartbeats from the signal. cpm, counts per minute; R–R interval, the time interval between two successive heartbeats, measured from one R-peak to the next in the ECG signal. Panel **b**, image courtesy of S.G. Panels **c** and **d** reprinted with permission from ref. 10, AAAS. Panels **e–g** reprinted from ref. 20, Springer Nature Limited.

Detection of middle-ear fluid using smartphones

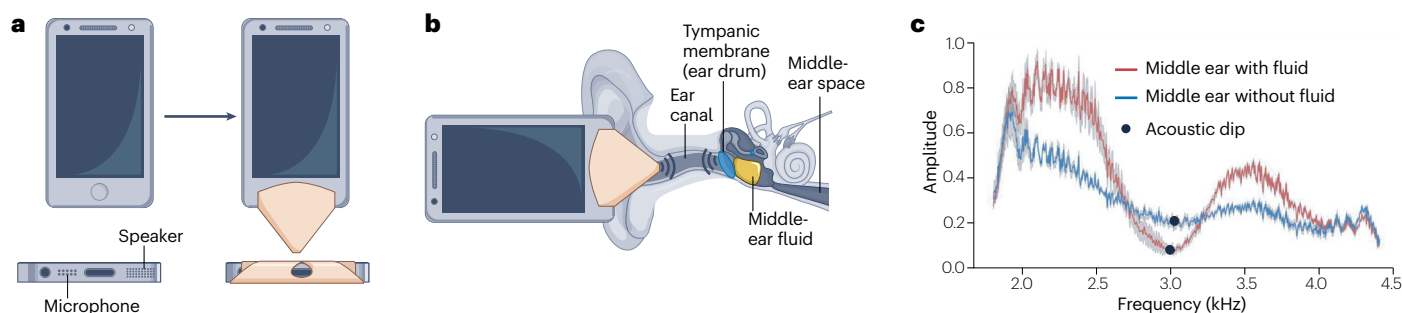

Newborn hearing screening using low-cost earphones

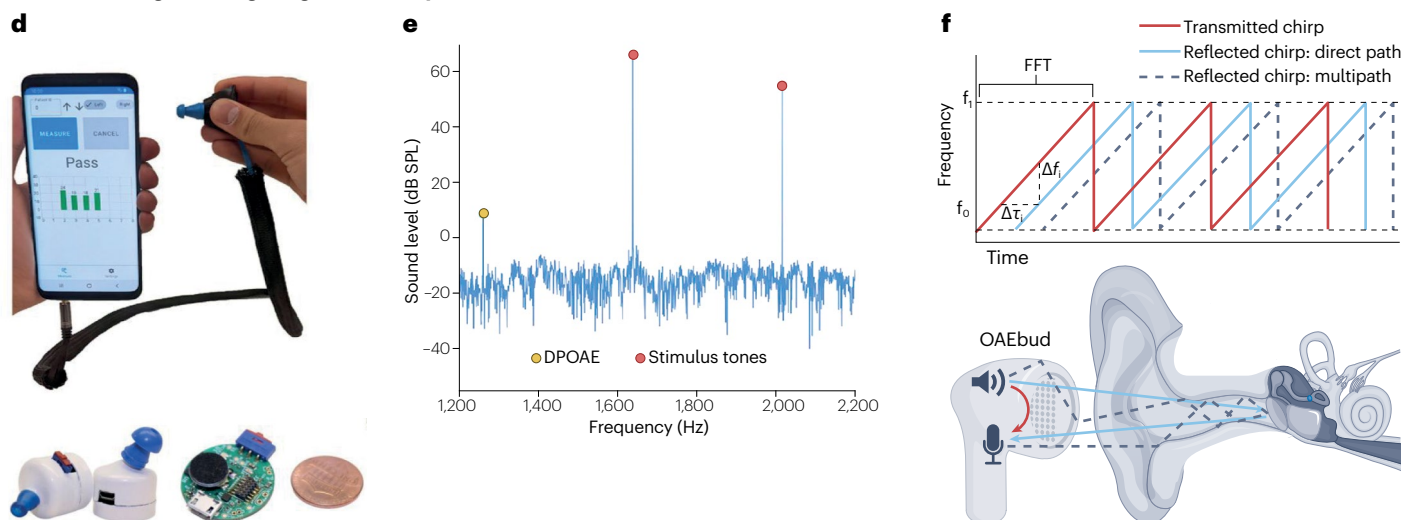


Fig. 3 | Low-cost earable systems to detect ear disorders. **a–c**, Middle-ear fluid can be detected using smartphones¹⁵. **a**, A paper funnel is attached to the phone, on which the speaker and microphone are co-located at the base. **b**, Active sonar is then applied to detect middle-ear fluid. **c**, Acoustic reflections from the ear differ depending on the presence of middle-ear fluid. **d–f**, Newborn hearing screening using low-cost earphones^{22–24}. **d**, Earphones and wireless earbuds can be applied to detect newborn hearing loss. **e**, Two stimulus tones f_1 and f_2 , are transmitted through each of the earbuds to stimulate the cochlea's hair cells. Using wireless sensing algorithms, the microphone detects the sounds of

vibrating hair cells, which is then used as a measure of hearing status. **f**, Wireless earbuds can eliminate unwanted reflections from the ear canal and eardrum using frequency-modulated continuous-wave radar (FMCW) processing to calculate the time of arrival of reflections from the ear canal. FFT, fast Fourier transform; DPOAE, distortion product otoacoustic emissions; OAEbud, otoacoustic emissions earbud; dB SPL, sound pressure level in decibels; Δf , frequency shift; $\Delta \tau$, time delay. Panels **a–c** reprinted with permission from ref. 15, AAAS. Panels **a–f** reprinted from ref. 24, Springer Nature Limited.

brightness changes that correlate with arterial pulse amplitude and blood pressure. The oscillometry principle can also be applied without requiring mechanical attachments¹⁸ by leveraging the smartphone's vibration motor and performing vibrometric force estimation using the onboard IMU.

Detecting disease. Colour-analysis systems can detect diseases from images captured by smartphone cameras. For example, BiliCam^{85,86} is a low-cost system that identifies jaundice in newborns by detecting yellow discolouration of their skin. Here, a colour-calibration card is used to standardize across different smartphones and lighting conditions, enabling bilirubin estimation, which is as accurate as when determined by blood tests and comparable to readings from

non-invasive bilirubinometers. BiliScreen⁸⁷ can identify subtle discolourations in eye images to detect mild, visually imperceptible forms of jaundice. The test is performed using either paper glasses with calibration markers to colour-balance across different lighting conditions or within the controlled lighting environment of a head-mounted display. Calibration-card-free visual detection of anaemia can be achieved using image metadata to normalize across lighting conditions⁸⁸. Smartphone images also allow the detection of eye conditions that typically require a specialized camera to capture retinal fundus photos. Using a deep learning model, these images can detect eye conditions, such as diabetic retinopathy and diabetic macular oedema, as well as poor blood-glucose control⁸⁹. CapApp⁹⁰ measures capillary refill time, which is the time taken by blanched

skin to return to its resting state after pressure has been applied. Here, a user presses their finger onto the camera of a vibrating phone and the amount of applied pressure is measured through dampened vibrations at the IMU, in addition to measurement of the brightness amplitude at the finger.

Scene-understanding systems

Cameras on extended reality devices, such as the HoloLens, heads-up displays and augmented-reality glasses have been explored for use in the operating room^{26–28}. For example, wearable camera systems can detect clinical medication errors by classifying drug labels on syringes and vials and flagging if labels might be mismatched, indicating an error²⁵. HoloLens can serve as an augmented reality-based system for surgical education to guide catheter placement into the brain ventricular system, a common neurosurgical procedure⁹¹. Video data captured from the egocentric point of view can also be applied for surgical tool detection and tracking to assess surgical skill^{92–95}. However, vision-based extended-reality systems rely on sampling from multiple high-resolution cameras, which requires high power and computational complexity to run machine learning models on streaming video data. Accurate and low-power scene-understanding systems would thus need to be optimized, including duty-cycling cameras, custom neural architecture designs and mechanisms to offload data to edge servers, while operating in real time.

Sensor fusion systems

Sensor fusion systems combine data from smartphones and wearable devices, such as smart watches and smart bands, to build a digital

phenotype of a user and infer their behavioural and physiological health states (Table 2). Such systems can also measure digital biomarkers that correlate with measures of mental health^{13,96–98}. Therefore, smart fusion systems allow for passive monitoring of the onset or progression of medical conditions over time. These systems typically leverage three main sources of data: passive sensor data, including IMU readings (accelerometer, gyroscope, magnetometer), global positioning system (GPS) location, network identifications and signal strengths (Wi-Fi and Bluetooth), ambient light, barometric pressure and skin temperature; digital activity traces, including call logs, internet browsing history, app usage and communication patterns (texts and emails); and questionnaires that periodically assess physiological, behavioural and mental state through tools such as ecological momentary assessment (EMA) and patient health questionnaires (PHQ). These sources of data can be applied to sense physical, behavioural and mental health conditions. To assess physical health, measurements can be combined across different built-in sensors, such as the IMU, or low-cost add-on sensors, such as electroencephalography (EEG) sensors, to obtain objective measures, such as blood pressure. Integrating multiple modalities can enable more accurate assessments. Behavioural health can be evaluated through inferences of raw sensor data to deduce digital phenotypes, such as activity and sleep patterns as well as indoor and outdoor mobility patterns, which are then correlated with measures of behavioural wellbeing, such as mood and loneliness, which can be obtained through questionnaires. Mental health monitoring relies on correlations between passive sensor data and digital activity traces to assess symptoms of conditions such as depression^{96,97} and schizophrenia^{13,99,100}.

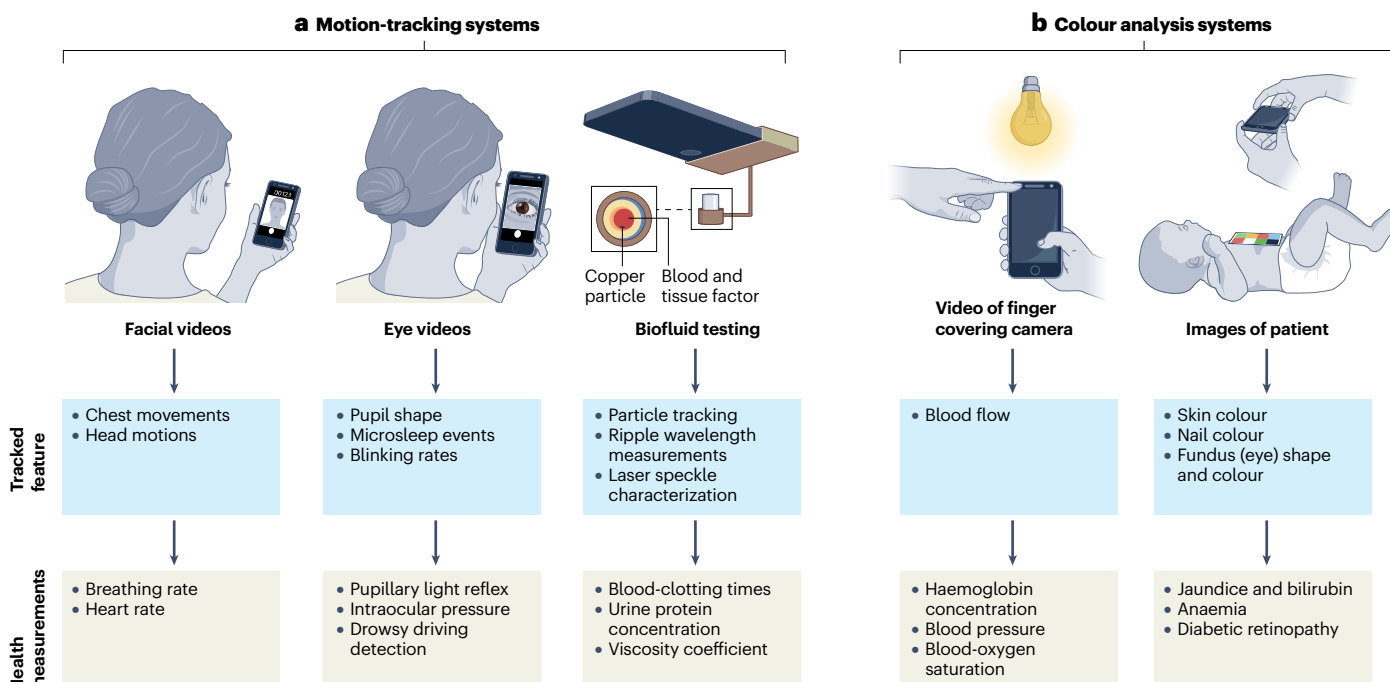


Fig. 4 | Vision-based systems. **a, b**, Vision-based systems leverage images and videos captured from the smartphone's front- or rear-facing camera. Computer vision algorithms based on motion tracking^{16,76,77} (**a**) or colour analysis^{78,85} (**b**) can be applied to measure physiological signals and health. Using motion-tracking algorithms, biofluid testing can be performed, for example, by tracking the

micro-mechanical motions of a copper particle in a vibrating sample of blood inside a plastic cup holder attached to a smartphone to measure clotting times¹⁶. Panel **a**, image courtesy of ACM, and adapted from ref. 71, CC BY 4.0 (<https://creativecommons.org/licenses/by/4.0/>), and reprinted from ref. 16, Springer Nature Limited. Panel **b**, image courtesy of Shwetak Patel.

Table 2 | Sensor fusion systems for behavioural health monitoring and digital phenotyping

Sensor	Digital phenotype	Digital traces	Medical findings
IMU	User activity (such as exercise level)	Call logs	Depression ^{12,14,96–98,123}
Microphone	Social interaction levels	Text messages, email patterns	Anxiety ⁹⁸
GPS	Outdoor mobility patterns	Internet browsing history	ADHD ¹²⁵
Wi-Fi and Bluetooth	Indoor mobility patterns	App usage	Schizophrenia symptoms ^{13,99,100}
Ambient light	Sleeping patterns		Mood ¹¹⁷
Camera	Event logging		Fatigue ¹⁴
Barometer	Elevation		Sleep quality ^{14,107}
Heat sensor	Body temperature		Stress ^{123,127}

ADHD, attention-deficit hyperactivity disorder; GPS, global positioning system; IMU, inertial measurement unit.

Physical health

Individual-scale sensing. The health outcomes of individuals with multiple sclerosis, including depression, fatigue, sleep quality and global symptom burden, in the stay-at-home period during the COVID-19 pandemic, could be predicted using smartphone sensor data (call logs, GPS location, screen activity), physiological data from a Fitbit activity tracker (step count, heart rate, sleep and wake times) and health questionnaire data¹⁴.

Earable systems can also exploit sensor fusion by using the onboard IMU and custom sensors to measure signals from the ear. For example, the IMU on the eSense^{101,102} earbud platform can measure and classify teeth grinding and clenching behaviour to detect bruxism¹⁰³. eBP¹⁰⁴ measures diastolic and systolic blood pressure from the ear canal using an in-ear air pump, pressure sensor and valve; here, pressure is applied to the outer ear canal by a microcontroller and an in-ear light-pulse sensor measures the PPG signal. WAKE¹⁰⁵ detects microsleep events using a custom earpiece to capture brain waves by EEG, eye movements by electrooculography (EOG), facial muscle contraction by electromyography (EMG), and skin conductivity by electrodermal activity. LIBS¹⁰⁶ measures brain activity, eye movement and muscle contraction using EEG, EOG and EMG signals, respectively, from an in-ear device. These signals are recorded as a single mixture and a signal-separation model is then applied to isolate individual signals and classify different sleep stages. EarSD¹⁰⁷ is an ear-worn system that enables the detection of epileptic seizures by sensing and classifying signals from EEG, EMG and EOG sensors.

Population-level sensing. The sensors of smart devices allow population-level sensing for public health and epidemiological surveillance. For example, digital-contact tracing^{108–110} can be used to track a user's exposure to individuals potentially infected with SARS-CoV-2 using smartphone sensor readings. Exposure is typically defined as being within a 1 m or 2 m range of an infected person¹¹¹. Although GPS location traces from a smartphone can provide **coarse-grained location estimates** with a distance resolution of 3–5 m, they do not provide sufficient accuracy to assess whether two people are within social distance. Furthermore, GPS cannot distinguish whether there is a wall or ceiling between two users and is thus unreliable indoors. Bluetooth-based solutions, such as TraceTogether¹⁰⁹ and **exposure**

notifications, rely on the received signal strength to infer proximity; however, such distance estimates might be unreliable. NOVID uses inaudible acoustic signals and time-of-flight ranging to measure the distance between smartphones. Smartphone clocks are able to measure the time down to milliseconds, and so the system can record when two phones have sent and received messages. By multiplying the difference between these timestamps with the speed of sound, NOVID produces a sub-metre distance estimate. However, in acoustic-based systems, signals can be attenuated by obstacles, and reflections can thus occur in a multipath-rich environment, which can interfere with the direct line-of-sight signal.

Global-scale datasets of passively measured accelerometer data have been analysed to reveal inequalities in the distribution of physical activity across different geographical regions, which might serve as a predictor of obesity prevalence. In addition, the walkability of a city might be associated with greater activity levels¹¹².

Behavioural health

Sensor fusion systems¹¹³ might also predict behavioural health based on passively sensed data. For example, SoundSense¹¹⁴ uses raw audio data from the microphone to coarsely classify sound into speech, music and ambient sound, which can then be more accurately divided into specific sound classes. These classified acoustic events can inform an audio diary of daily events, recorded over time. Moreover, sleep duration can be assessed according to smartphone usage patterns, recharge events, ambient light sensor data and accelerometer data¹¹⁵. However, continuous data sampling from multiple power-demanding sensors (particularly if the device is not charging) can substantially drain battery life. To address this challenge, JigSaw¹¹⁶ contains power-efficient pipelines to adaptively adjust sensor sampling rates; here, algorithms are applied to measure user activity speed from accelerometer data and accordingly to adjust the GPS sampling rate. An activity classifier is then applied to the raw accelerometer data to enable users to track their daily calorie expenditure and carbon footprint. The mood-sensing system MoodScope¹¹⁷ takes an alternative approach by relying solely on digital traces of smartphone usage patterns (app usage, website browsing behaviour, email, text message and phone call patterns as well as location data) to make inferences about a user's behaviour.

Sensor fusion systems can also promote positive changes to user behaviour. For example, BeWell^{118,119} applies quantitative scores to indicate whether a user is averaging adequate levels of sleep, aerobic activity and social interaction per day. These scores are presented to the user on their smartphone lock screen to promote wellbeing. MyBehavior¹²⁰ combines passively sensed data with manual logging of food intake and exercise patterns to provide personalized suggestions for calorie loss. UbiFit¹²¹ leverages accelerometer and barometer data to classify a user's physical activities, which are presented on the display to encourage exercise. The SmartGPA¹²² system measures a user's studying and socializing patterns to predict academic grade point average (GPA) performance, which could enable timely interventions for improving academic performance.

Mental health

The long-term mental health trends of populations might be assessed by smart sensor systems. For example, the digital phenotyping system StudentLife¹² has been applied to conduct a behavioural health study in a class of college students over the period of a school term. The system captured activity information (stationary, walking, running, driving, cycling) from IMU data, outdoor mobility patterns from GPS

samples, indoor mobility patterns from Wi-Fi scan logs, conversation levels from the microphone audio stream, sleep duration from ambient light readings and phone usage logs. Here, sensor data correlated with measures of mental wellbeing (depression, stress, flourishing, loneliness), which was assessed through user questionnaires. Several systems have focused on further understanding the dynamics and effects of depression in the college population^{96,97}.

Features could be developed on the basis of passively sensed data that relate to depression symptoms, as defined in the *Diagnostic and Statistical Manual of Mental Disorders*, 5th edition (DSM-5)⁹⁶. These features correlate with self-reported Personal Health Questionnaire depression scale PHQ-8 and PHQ-4 scores. Data from smartphones and fitness trackers can further be used to identify depression symptoms without requiring periodic recalibration, using ground-truth questionnaires⁹⁷. Here, depression scores are measured once at the beginning and once at the end of the semester, revealing post-semester depression 11–15 weeks before the end of the semester, thus allowing pre-emptive intervention. In a smartphone and ecological momentary assessment study, biomarkers of depression ($P = 0.03$) and anxiety ($P < 0.001$) in college students were found to statistically significantly correlate with fluctuations in COVID-19-related news during the COVID-19 pandemic⁹⁸. Similar patterns have been identified in other populations¹⁴.

Digital phenotyping systems can also be applied in clinical studies to remotely assess new quantitative biomarkers in individuals with medical and psychiatric conditions^{123,124}. For example, LemurDx^{125,126} uses smartwatch accelerometer data to measure increased hyperactivity from hand motion, which could indicate an attention-deficit hyperactivity disorder (ADHD). Trained with coarse activity information about children, provided by parents at the end of the day, the system can classify different activity patterns (sleeping, sitting, household activity, exercise, not wearing a watch). These motion data can then be combined with location data from GPS, a heart rate sensor on the smartwatch and Bluetooth scans.

CrossCheck^{13,99} and an approach using encoder–decoder neural networks¹⁰⁰ can predict the severity of psychiatric symptoms in individuals diagnosed with schizophrenia (seeing things, hearing voices, worrying about being harmed) to aid in disease monitoring and preventing relapse. Digital phenotyping systems¹²⁷ have also been evaluated in a population of resident physicians, which are at risk of workplace stress and developing mental health symptoms, identifying physiological indicators of stress-resilience from physical activity, sleeping behaviour, heart rate and mood.

Custom low-cost sensing systems

In addition to mobile systems that make use of onboard sensors and smart devices, custom low-cost sensing systems enable alternative forms of healthcare monitoring. Furthermore, mobile medical systems allow large-scale digital epidemiology in the form of contact tracing.

Wearable sensing systems

Joey¹²⁸ is based on a conductive fabric necklace that can measure the heart and respiration rate of infants through ECG signals during kangaroo mother care (chest-to-chest skin contact between the infant and a caregiver). Here, diffusion-based denoising models disentangle the ECG signals from the caregiver and the infant. PPG sensors, usually used in pulse oximeters and wearable devices to estimate heart rate, blood-oxygen saturation and other physiological parameters, provide less accuracy in individuals with dark skin because their higher

melanin levels affect the absorption of laser light. MagWear¹²⁹ tackles this issue by leveraging biomagnetism to measure heart rate and respiratory rate through a small magnet at the wrist. The magnet pushes blood flow, and biomagnetic field signals are then induced thanks to the ions produced by each heartbeat. This can be measured with a giant-magnetoresistance sensor. Painometry¹³⁰ relies on a hat-shaped form factor sensing platform that measures EEG, PPG and galvanic skin response to objectively quantify a user's pain perception. Custom smart rings^{131–133} with integrated IMU and PPG sensors might also be applied to monitor heart and respiration rate.

Instrumenting health devices

Health devices can be equipped with additional sensors to enrich health monitoring. For example, ToMoBrush¹³⁴ can be applied to electric toothbrushes, using microphones to extract the acoustic resonance of an individual tooth and assess its dental condition. IOTeeth¹³⁵ integrates piezoelectric sensors in a dental retainer platform to monitor dental occlusal diseases, which can result in tooth loss, by tracking teeth biting and grinding activities. MechanoBeat¹³⁶ can be applied to create 3D-printed tags that oscillate at a distinct frequency, which can be sensed with an ultra-wideband radar array to detect when a user interacts with a medicine pill bottle. Similarly, an insulin pen can track the number of times insulin is dispensed¹³⁷.

Real-world challenges

Mobile health systems should work in different environments and for smart devices from different manufacturers. They should also be designed to mitigate biases and ensure trust, which requires policies enforced by regulatory bodies. Moreover, mobile health systems need to be integrated with clinical care processes.

Scaling to real-world environments

Deploying mobile medical systems in real-world environments faces challenges that are typically not seen in the controlled environments they were initially prototyped in.

Uncontrolled environments. Real-world testing environments can be complex, with suboptimal testing conditions, such as different levels of background noise and ambient lighting conditions, as well as human motion. Therefore, systems need to be designed to detect and tolerate real-world conditions. For example, smartphone-based systems that can detect opioid-induced depressed breathing require filters to remove audible environmental noise and distinguish breathing from other body motions¹⁰.

Dataset collection. Scaling to multiple environments might require the collection of large amounts of diverse data, which can be costly and difficult. Efficient dataset collection approaches, such as crowdsourcing, and data-augmentation methods to create synthetic datasets, enable scaling across a large number of environments. For example, to collect breathing sounds from different smartphones and environments, the Amazon Mechanical Turk crowdsourcing platform has been harnessed to recruit individuals, who recorded their sleep with their smartphone microphone²⁹. These recordings were subsequently used to train generative artificial intelligence (AI) models, such as generative adversarial networks, to produce synthetic data.

Data heterogeneity and incompleteness. Sensor fusion systems, such as those used for digital phenotyping, measure data from multiple

sensor modalities (for example, IMU, microphone, light sensor, network signal strength), digital activity traces (for example, app usage levels, texting behaviour) and data types (for example, time series, survey results, symptoms). Machine learning models are typically designed to work with a single data type and cannot easily integrate heterogeneous data streams¹³⁸. Multimodal machine learning models aim to jointly learn from different data types, which requires addressing challenges in data representation, translation, alignment, fusion and co-learning¹³⁹. Furthermore, they cannot easily deal with data that are missing, incomplete or noisy, which can be produced by sporadic and uncontrolled usage patterns¹³⁸. Therefore, data cleaning and preprocessing, in the form of noise and outlier removal, as well as data interpolation¹³⁸, are typically required before machine learning models can be used.

Generalizing to diverse hardware designs

Medical devices are typically purpose-built for a standardized hardware design, which often differs from that used in smart devices and sensors. Furthermore, sensors, such as microphones and speakers, can degrade in quality over time. To address this, new clinical data can be collected for each new device; however, this approach can be time-consuming or infeasible, given the diversity of newly launched devices.

Sensor-calibration techniques, such as colour-coded reference cards^{85–87} and image metadata⁸⁸, can be applied to normalize colour profiles for images captured across different smartphone cameras. A standardized acoustic cavity can be used to calibrate the acoustic frequency response of a speaker and microphone²⁴, which allows scaling of new devices without the need to collect additional clinical data. Systems that leverage the IMU for tasks, such as step counting, rely on features such as normalized auto-correlation, which work across different accelerometer sensitivities and sampling rates^{140,141}.

However, not all hardware sensors can be calibrated by the user upon use. For example, in the case of contact-tracing apps that rely on Bluetooth signal strength to determine whether two smartphones are close to each other, each smartphone model might have a different Bluetooth radio chip, antenna layout and phone operating system version, which could report different readings for the same distance. Obtaining the per-phone mapping from the received signal strength indicator to distance typically requires manual readings collected in an anechoic chamber, which is a time-consuming procedure. **Trace-Together**, a Bluetooth-based contact tracing system, can perform this manual calibration process.

Mitigating bias from sensor-based systems

Medical mobile systems that do not address clinical bias can perpetuate health inequities. For example, systemic biases can be propagated in systems that are trained with chest X-ray images¹⁴², diabetic retinopathy fundus images¹⁴³, clinical interviews and records¹⁴⁴ and other medical records¹⁴⁵. Therefore, the FDA has released an **action plan** with the aim of supporting improvements to models after deployment. Bias might be mitigated through the generation of synthetic data by generative AI systems¹⁴⁶, such as generative adversarial networks¹⁴⁷, variational autoencoders¹⁴⁸ and large language models, particularly for under-represented disease classes or severe disease states^{149–151}. Synthetic data can also be generated using physics-based simulations in silico or benchtop models in vitro^{152–154}.

Gender bias. Women and men show differences in ECG parameters during adolescence, with women typically having a faster heart rate

compared to men and differences in QT interval (ventricular depolarization and repolarization time), QTc interval (heart rate-corrected QT) as well as QRS complex (ventricular depolarization amplitude and duration) owing to hormonal differences. These differences can result in greater levels of risk for certain diseases, with women aged 20–40 having a threefold greater risk of arrhythmic-related cardiac events compared with men¹⁵⁵. Mobile ECG systems can show reduced accuracy in women if they are trained primarily on data from men, which might lead to increased false positives for women in the ECG-based diagnosis of ischaemia¹⁵⁶. This gap might be partly addressed by increasing awareness during medical training and by adapting models to physiological differences.

Women and men also differ in their gait – for example, in kinematic and kinetic variables in both healthy individuals and those with osteoarthritis^{157,158}, which can be applied for automatic gait-based sex classification¹⁵⁹. These differences should be accounted for in mobile medical systems, particularly in those performing activity recognition, through a balanced dataset or by incorporating sex-specific gait features into machine learning models to reduce bias.

Age bias. Mobile medical systems that measure physiological signals such as PPG and blood pressure should consider age-related physiological differences. The PPG waveform at the ear, finger and toes changes with age owing to differences in physiology¹⁶⁰. In particular, increased arterial stiffness might affect key signal features in the PPG waveform of older individuals, making them more challenging to detect¹⁶¹. Pulse oximetry measurements leveraging PPG can be biased owing to motion artefacts, for example, in children. Therefore, large probes should be adapted to the small fingers of neonates and infants, and devices should be calibrated with data from healthy young adults¹⁶². Moreover, age-matched ranges should be used in the evaluation of individuals with vascular disease¹⁶⁰. Blood-pressure measurements are considerably affected by age, with systolic blood pressure being increasingly underestimated and diastolic blood pressure being increasingly overestimated with increasing age, compared to invasive aortic blood-pressure measurements¹⁶³. Therefore, personalized blood-pressure measures are required to normalize for age.

Skin-tone bias. Wearable sensing systems measuring arterial oxyhaemoglobin saturation by pulse oximetry perform worse in individuals with darker skin tones compared to those with lighter skin tones, owing to differences in skin absorption and scattering characteristics influenced by melanin levels^{164,165}. The calibration parameters of these devices are often biased towards individuals with lighter skin tones¹⁶⁶, and inaccuracies in pulse oximetry measurements can result in the under-detection of hypoxia and sleep apnoea^{167,168}. Importantly, such measurements are used by insurance companies to determine eligibility for medical reimbursement, and thus, systemic errors in pulse oximetry measurements can further promote inequities in healthcare.

The low performance of PPG on darker skin can be addressed by the MagWear system¹²⁹. Similarly, inaccurate pupillometry results in individuals with darker irises can be addressed through the use of a smartphone-based filter to perform the test in the far-red visible light spectrum⁷².

Cultural bias. Mobile systems that rely on speech detection and transcription to assess mental health may perform poorly on a diverse range of accents if primarily trained on a single accent^{169,170}. Speech-based health-sensing systems that rely on vocal prosody to detect mood

may function differently for English compared to tonal languages, such as Mandarin^{169,170}. Digital phenotyping systems may leverage psychological models of stress, anxiety and depression, which cannot be generalized across cultures¹⁷¹. Diet-tracking systems for individuals with diabetes are often optimized for specific diets and may thus inaccurately estimate the glycaemic response to diverse foods¹⁷². Moreover, religious headwear should be accounted for in systems that require head-mounted sensors, such as EEG sensors or heads-up displays¹⁷³.

Medical history bias. Pre-existing medical conditions can act as a confounding factor, affecting the accuracy of sensing technologies. For example, arrhythmias and irregular heart rhythms affect the shape of the PPG waveform and can affect measurements of heart rate, heart rate variability and blood-oxygen saturation¹⁷⁴. Diseases that affect movement, such as Parkinson's disease, can result in motion artefacts in PPG waveform measurements. Medications can also introduce biases; for example, beta-adrenergic-blocking drugs can increase heart-rate variability¹⁷⁵; endocrine medications for thyroid disease can affect drug metabolism¹⁷⁶; and psychiatric medications, such as selective serotonin reuptake inhibitors and antidepressants, affect the heart rate¹⁷⁷ and can cause sleep disorders, such as apnoea and bruxism¹⁷⁸. Such medication-induced variations can lead to false-positive or false-negative readouts in medical devices that monitor sleep or cardiac conditions. Therefore, patient-specific calibration protocols and alternative sensing modalities might be required.

Digital literacy bias. Lack of or limited literacy of users and/or healthcare professionals as well as limited implementation of electronic health record systems can negatively affect the effectiveness of mobile medical systems^{179–181}. This might be addressed by providing user interfaces and instructions that rely on graphics, video and voice guidance. By integrating mobile medical systems into the continuum of care, provider-assisted onboarding and training can also help to increase adoption of these systems. In addition, public health policies to increase access to computing devices and training on digital health technologies might promote the deployment of digital health systems.

Trust in mobile health systems

Establishing trust is an important factor in the deployment of mobile health systems. Sensors in mobile health systems can capture sensitive data beyond health information. For example, cameras and microphones might capture sensitive and identifiable data, such as the user's face, surrounding environment, data from bystanders^{61–68} and voice data³⁸. Although privacy concerns might be partly addressed by technological mitigation strategies, such as data processing at the edge, data obfuscation, filtering and anonymization, data leaks, unauthorized access and data exploitation remain concerns¹⁸².

Maintaining patient privacy

Built-in privacy-preserving technologies can minimize data leakage while maintaining device performance.

Edge computing. Mobile medical systems that rely on machine learning models to process sensor data might send data to the cloud for further processing, which bears the risk of data being compromised in transit or at the server. Running algorithms and models on an edge computing device, such as smart devices, mobile central processing units and mobile graphics processing units, can help to preserve patient privacy. However, the model has to be optimized for the constrained

computational resources of mobile or embedded devices, while maintaining a high level of clinical accuracy. Optimization techniques, such as pruning¹⁸³, quantization¹⁸⁴, knowledge distillation¹⁸⁵, model compression¹⁸⁶, low-rank factorization¹⁸⁷ and neural architecture search¹⁸⁸, can help to reduce model size, inference time and memory footprint to enable deployment on edge devices.

Federated learning. By re-training a model with new patient data using federated learning^{189,190}, local models can be trained on edge devices, and only encrypted model updates are sent to a central server, where they are aggregated. An updated model is then sent back to the local devices. This strategy allows hospitals to comply with privacy regulations, such as the Health Insurance Portability And Accountability Act (HIPAA) and the General Data Protection Regulation (GDPR), by ensuring that patient data stays within the institution¹⁹¹.

Privacy-preserving techniques can also be designed at the hardware level; for example, inaudible frequencies can be used in sensors that assess behavioural biomarkers in digital phenotyping systems¹⁹², or depth or thermal cameras can be applied instead of RGB cameras for vision-based systems⁵⁰. At the software level, secure enclaves and homomorphic encryption can be used¹⁹³.

Improving explainability

Black box machine learning models, for which the underlying mechanistic information is lacking, might also compromise trust. For patients, intuitive and non-technical (plain language) explanations and colour-coded risk scores can increase the accessibility of medical information¹⁹⁴. In addition, generative AI can create synthetic medical images for patient education¹⁹⁵. Healthcare personnel can benefit from saliency maps¹⁹⁶ that highlight relevant regions in a medical image to help them to understand a model's focus and build trust in the system. Similarly, concept-based explanations can translate a model's prediction into familiar medical concepts¹⁹⁷. Concept activation vectors¹⁹⁷ can be used in the diagnosis of diabetic retinopathy from retinal fundus images¹⁹⁸, providing a score for different diagnostic concepts, which might help in the interpretation of a model's predictions and flag instances in which healthcare professionals disagree with the model.

Shapley values¹⁹⁹ quantify how much each feature contributes to a model's prediction. For example Prescience²⁰⁰ uses Shapley values to provide a numeric representation of hypoxaemia risk (odds ratio) and quantify the contribution of pulse level, tidal volume, body-mass index and other factors to the prediction. Local interpretable model-agnostic explanations²⁰¹ allow physicians to assess how perturbations to these different features affect the model's predictions and whether the model's responses align with their medical knowledge.

Building trust with patients and the public

The integration of mobile medical systems into clinical workflows and endorsement by healthcare professionals and institutions can increase a patient's trust. Ensuring compatibility with electronic health record systems and telemedicine platforms can further facilitate adoption and reinforce the credibility and reliability of systems. Patient-provider interactions are also important in building trust through face-to-face interactions, training and guidelines for standardized use¹⁸². Moreover, deployment by reputable service providers, publications and endorsements increase trust¹⁸², in addition to compliance with data privacy regulations, such as HIPAA and GDPR, as well as cybersecurity certifications, such as ISO 27001 for data security^{202–204}.

Sociodemographic factors can affect a patient's trust in a mobile medical system. Systems which are difficult and cumbersome to use can negatively affect a user's confidence in digital health technologies and their effectiveness²⁰⁵. Intuitive user interfaces with clear graphics and videos, multilingual support and customer service hotlines for personalized training can increase access and accommodate a range of users^{182,206}. Moreover, users can be provided with granular control over data collection, storage and sharing capabilities by enabling opt-in permissions and consent, the ability to delete stored data and explicit requests for data sharing. In addition, real-time privacy indicators, such as status lights when a system is collecting data, can reduce uncertainty about unauthorized recordings^{207,208}.

Users should also be provided with a channel to report concerns about system performance and shortcomings, such as feedback forms to report false-positive or false-negative results. Periodic software updates to algorithms, models and security architecture can also increase trust and system reliability.

Regulatory considerations

Mobile medical systems face distinct regulatory challenges, including variability in hardware sensors and software application programming interfaces across different models.

Software as a medical device quality management system

The hardware in mobile medical systems is not considered a medical device hardware. The FDA provides regulatory guidance for mobile medical systems that leverage sensors on smart devices. The [guidance for mobile medical applications](#) and [software as a medical device](#) (including the quality management system and the requirements for production engineering) regulates the custom software application, not the hardware of smart devices, which reduces the costs for regulatory clearance. The [FDA has approved mobile medical systems that leverage device sensors](#), such as microphones and cameras; for example, [sonar-based breathing monitors](#) using a smartphone or smart speaker have obtained FDA clearance under software-as-a-medical-device guidelines and via the 510(k) pathway.

According to the [medical device academy](#) (a quality and regulatory consulting firm for FDA 510(k) submissions) the cost of human clinical studies, which is required in only 10% of 510(k) submissions, ranges from US\$250,000 to US\$2.5 million. Simple clinical studies can cost less than US\$100,000, whereas for mobile medical apps, which may only consist of software and fall under the software-as-a-medical-device guidelines, the testing costs might be lower.

Calibrating new mobile medical systems

The calibration of a new vision-based mobile medical system can be achieved with colour-calibration cards. For example, the urinalysis app [MinuteKidney](#) is an FDA-cleared class II medical device that uses a colour-calibration card. Users take a picture of a urinalysis dipstick against a colour-calibration card using a smartphone camera, and computer vision techniques take into account the camera's colour profile and ambient lighting conditions to calibrate the captured image, enabling its application across different smartphone models and operating systems.

External attachments

Mobile health systems that rely on external components – such as 3D-printed parts, paper-based tools requiring user assembly or a colour-calibration card that needs to be printed on paper or displayed

on a screen – necessitate a regulatory strategy that determines whether the system is considered a finished or unfinished medical device. Unfinished medical devices introduce variability in the assembly process, which can affect system performance and requires clear instructions and user testing. Alternatively, pre-fabricated and pre-assembled components can be provided to improve reliability and facilitate classification as a finished medical device.

Different operating system versions

Software applications that are built against the Android SDK (version 29 and above, which is supported on Android 10 OS) are designed to be compatible with future versions of Android, as indicated in the [Android API](#) documentation. The SDK is designed to isolate applications and extensions to the Android OS, allowing app compatibility with future OS updates. In the case of iOS or other mobile operating systems, calibration procedures may need to be created to ensure that sensor readings can be interpreted across different OS versions and to mitigate the effect of changes to sensor application programming interfaces.

Clinical integration and automated interventions

Integration with the clinical continuum of care

Medical findings obtained by mobile medical systems need to be considered within the context of clinical care by integrating device readouts with medical records to facilitate informed decision-making. However, this requires electronic medical records that allow interoperability and adhere to data standards. For example, formats such as fast healthcare interoperability resources, to transfer data from mobile health systems to electronic health records, enable integration into clinical workflows²⁰⁹. Partnerships with public health authorities, healthcare administrators, insurance companies and other key stakeholders may be needed to ensure inclusion of these findings in the medical record. Engaging with insurance companies to ensure a mobile medical test will be reimbursed using an existing or new current procedural terminology code might further promote their integration and adoption²¹⁰.

Mobile medical systems could support the initial stages of the continuum of care by enabling the remote screening, diagnosing or monitoring of a medical condition. However, clinical oversight is important to ensure that the test is performed correctly and the result is interpreted within the context of a patient's medical history and demographics, so that guideline-based interventions, personalized treatment plans and rehabilitation and therapy can be implemented appropriately. Therefore, mobile medical devices might not only increase access to healthcare but also aid in timely clinical decision-making without requiring a face-to-face consultation.

Closed-loop systems

Closed-loop systems can interpret measurements and automatically initiate clinical interventions. For example, a [fall detection](#) feature on a smart watch uses onboard motion sensors to detect and initiate an alarm if the user has fallen, automatically contacting emergency services and contacts. In a [car crash detection](#) feature, motion sensors detect severe car crashes, automatically calling emergency services if the user does not respond to a system-initiated alert. The Pixel Watch 3 includes a [loss of pulse detection](#) feature that automatically calls emergency services if the user's heart has stopped beating. [Wristbands](#) have been FDA-cleared for the detection of generalized tonic-clonic seizures for patients with epilepsy, alerting caregivers or emergency contacts.

The Apple watch and FitBit watch also have features that do not strictly meet the definition of a closed-loop system, but provide a basic form of clinical interpretation; for example, the [irregular heart rhythm](#) feature and [ECG app](#) alert the user in the case of rhythms indicating atrial fibrillation, suggesting that a doctor be consulted.

In addition, an active-sonar system can be applied to detect opioid-induced respiratory depression¹⁰ to initiate the injection of naloxone and thus reverse an opioid overdose²¹¹. Moreover, passive acoustic sensing systems might be applied to detect biomarkers, such as agonal breathing²⁹, to initiate contact with emergency services that can then perform cardiopulmonary resuscitation.

Outlook

Ensuring that timely in-person appointments with clinicians take place can be difficult in low-resource settings and rural areas. Mobile medical devices might expand access to health assessments. [Mobile medical apps](#) that leverage smartphone sensors for health sensing have received FDA clearance, demonstrating that smartphones can be used as a platform for healthcare delivery and to reduce health inequities. In addition, smart speakers, smart watches, wireless earbuds and smart eyewear can be applied to the continuous monitoring of emergent conditions such as cardiac arrests²⁹ and mental health problems^{12,98,123}, the ambient monitoring of surgeries and drug preparation in the operating room^{25,212}, and hearing-loss screening in low- and middle-income countries^{23,24}.

Various mobile medical systems that rely on built-in sensors of smart devices for health assessments have already passed regulatory clearance or are commercially available. For example, the [active sonar technology for smartphones](#) was FDA-cleared in 2021 as a respiratory monitoring app. This technology is also used by the [SleepScore app](#) to provide an index of sleep quality. The Pixel 8 Pro smartphone leverages an infrared sensor to measure body temperature at the forehead, and is the first [FDA-granted smartphone app for body-temperature monitoring](#), classified under the ‘de novo’ category. A smartphone’s thermister can also be applied to measure body temperature across different smartphone models²¹³. The [Google Fit app for Pixel phones](#) relies on computer-vision techniques to measure respiratory rate from the front-facing camera by examining small movements of the chest, as well as heart rate by placing a finger on the rear-facing camera and tracking subtle changes in colour. The [Digital Wellbeing app](#) checks coughing and snoring activity using passive acoustic sensing to detect the distinct acoustic fingerprints associated with these body sounds. [Sleep sensing algorithms](#) have also been integrated into smart devices. For example, Nest Hub devices leverage mmWave radar to detect an individual’s movement, and measures sound, light and temperature to assess sleep quality by machine learning. Fitbit uses the heartbeat and IMU signal to estimate sleep stage. The Apple Watch and Pixel Watch apply motion sensors for car crash detection, fall detection and loss of pulse detection. The Apple Watch and FitBit watch also have an ECG sensor for detecting [irregular heart rhythms](#) suggestive of atrial fibrillation. The Samsung Galaxy Watch can measure [body composition](#) (body-fat percentage, body-water content, skeletal muscle mass) using bioelectrical impedance analysis. The watch can also measure [blood pressure](#) using the onboard PPG sensor. Smart rings, such as the Oura Ring, can monitor [heart rate](#) and [blood oxygen](#), and measure body temperature to [predict the start of the menstrual period](#).

In addition, mobile medical systems might have an impact in telemedicine, precision healthcare, long-term health monitoring and disease detection.

Expanded medical tests for telemedicine visits

Healthcare can be made more accessible by increasing the number of medical tests that can be performed remotely through a telemedicine appointment and mobile medical systems^{214,215}. For example, mobile medical systems might enable low-cost ultrasound imaging, vital-sign monitoring of a fetus and biofluid testing. However, they require a similar level of accuracy to in-clinic assessments, allow untrained users to perform the test, provide results that are interpretable by both the patient and healthcare provider and protect patient privacy.

Small-data mobile systems for precision healthcare

Machine learning systems for medical diagnostics are typically built on large datasets that should represent the entire population. For example, speech-recognition technology requires training with a variety of words, phrases and accents. However, this would require mobile systems that can be fine-tuned using orders-of-magnitude less data than current systems, for example, by applying few-shot- or zero-shot-based learning methods.

Ambient sensing systems for long-term health monitoring

Smartphones, smart watches and smart speakers might also enable long-term continuous monitoring; for example, ambient monitoring systems can track medical events over time in a contactless manner. Such ambient sensing systems could also be designed to detect recurring events, such as seizures, and to learn from an individual’s distinct physiological patterns to become more accurate. In addition, these systems can leverage audible biomarkers to track long-term changes in vocal patterns and measure the progression of cognitive disorders, such as dementia and Alzheimer’s disease. However, they need to be privacy-preserving.

Sensors for disease detection

Dogs and insects can smell diseases, such as COVID-19 (ref. 216), diabetes²¹⁷ and cancer^{218–220}. However, even the best electronic sensors are substantially less sensitive than biological sensing systems. Biomimetic electronic or biohybrid sensors that can detect the presence of disease from gaseous chemical compounds in breath or scent²²¹, with the help of machine learning algorithms, could be integrated into mobile and non-invasive diagnostic tools, for example, to track the health of individuals in public spaces or to create a real-time barometer of a city’s health and track the outbreak of diseases.

Published online: 3 July 2025

References

1. World Health Organization. Local production and technology transfer to increase access to medical devices — addressing the barriers and challenges in low- and middle-income countries; <https://www.who.int/publications/i/item/9789241504546> (2012).
2. Diaconu, K. et al. Methods for medical device and equipment procurement and prioritization within low- and middle-income countries: findings of a systematic literature review. *Glob. Health* **13**, 59 (2017).
3. Vasan, A. & Friend, J. Medical devices for low- and middle-income countries: a review and directions for development. *J. Med. Devices* **14**, 010803 (2020).
4. Haile, L. M. et al. Hearing loss prevalence and years lived with disability, 1990–2019: findings from the Global Burden of Disease Study 2019. *Lancet* **397**, 996–1009 (2021).
5. Hay-McCutcheon, M. J., Threadgill, M., Yang, X. & Phillips, F. Access to hearing health care, geographical residency, and quality of life in adults with and without hearing loss. *J. Am. Acad. Aud.* **31**, 485–495 (2020).
6. Singer, D. E. et al. Impact of global geographic region on time in therapeutic range on warfarin anticoagulant therapy: data from the ROCKET AF clinical trial. *J. Am. Heart Assoc.* **2**, e000067 (2013).
7. Mwita, J. C. et al. Quality of anticoagulation with warfarin at a tertiary hospital in Botswana. *Clin. Appl. Thromb.* **24**, 596–601 (2018).

8. Semakula, J. R. et al. A cross-sectional evaluation of five warfarin anticoagulation services in Uganda and South Africa. *PLoS ONE* **15**, e0227458 (2020).
9. Nandakumar, R., Gollakota, S. & Watson, N. Contactless sleep apnea detection on smartphones. In *Proc. 13th Ann. Int. Conf. Mobile Systems, Applications, and Services* 45–57 (ACM, 2015).
This article reports a smartphone-based system that detects sleep apnoea events using its built-in speakers and microphones as an active sonar to track subtle chest movements.
10. Nandakumar, R., Gollakota, S. & Sunshine, J. E. Opioid overdose detection using smartphones. *Sci. Transl. Med.* **11**, eaau8914 (2019).
11. Larson, E. C., Lee, T., Liu, S., Rosenfeld, M. & Patel, S. N. Accurate and privacy preserving cough sensing using a low-cost microphone. In *Proc. 13th Int. Conf. Ubiquitous Computing (UbiComp '11)* 375–384 (ACM, 2011).
This article reports a privacy-preserving cough detection system that uses mobile phone microphone audio while ensuring speech cannot be reconstructed intelligibly.
12. Wang, R. et al. StudentLife: assessing mental health, academic performance and behavioral trends of college students using smartphones. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 3–14 (ACM, 2014).
This article reports a smartphone-based passive sensing app that continuously measures how workload affects stress, sleep, activity, mood, sociability, mental well-being and academic performance in a college student population.
13. Wang, R. et al. CrossCheck: toward passive sensing and detection of mental health changes in people with schizophrenia. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 886–897 (ACM, 2016).
14. Chikeral, P. et al. Predicting multiple sclerosis outcomes during the COVID-19 stay-at-home period: observational study using passively sensed behaviors and digital phenotyping. *JMIR Ment. Health* **9**, e38495 (2022).
15. Chan, J., Raju, S., Nandakumar, R., Bly, R. & Gollakota, S. Detecting middle ear fluid using smartphones. *Sci. Transl. Med.* **11**, eaav1102 (2019).
This article reports a smartphone-based system that detects middle-ear fluid using its built-in speakers and microphones to assess eardrum mobility, and a paper funnel to channel sound in and out of the ear canal.
16. Chan, J., Michaelsen, K., Estergreen, J. K., Sabath, D. E. & Gollakota, S. Micro-mechanical blood clot testing using smartphones. *Nat. Commun.* **13**, 831 (2022).
17. Goel, M. et al. Spirocall: measuring lung function over a phone call. In *Proc. Conf. Human Factors in Computing Systems (CHI '16)* 5675–5685 (ACM, 2016).
This article reports a system that enables spirometry on the phone using the standard telephony voice channel to transmit the sound of spirometry; this system can operate with or without a 3D-printed vortex whistle.
18. Barry, C., Xuan, Y., Fascetti, A., Moore, A. & Wang, E. J. Oscillometric blood pressure measurements on smartphones using vibrometric force estimation. *Sci. Rep.* **14**, 26206 (2024).
19. Wang, A., Sunshine, J. E. & Gollakota, S. Contactless infant monitoring using white noise. In *25th Ann. Int. Conf. on Mobile Computing and Networking (MobiCom '19)* 52 (ACM, 2019).
20. Wang, A., Nguyen, D., Sridhar, A. R. & Gollakota, S. Using smart speakers to contactlessly monitor heart rhythms. *Commun. Biol.* **4**, 319 (2021).
This article reports a smart speaker-based system that uses active sonar to detect individual heartbeats and measure heart rate as well as inter-beat intervals for both regular and irregular rhythms.
21. Chan, J. et al. Performing tympanometry using smartphones. *Commun. Med.* **2**, 57 (2022).
22. Ali, N. et al. An open-source smartphone otoacoustic emissions test for infants. *Pediatrics* **6**, e2024068068 (2025).
23. Chan, J. et al. Wireless earbuds for low-cost hearing screening. In *Proc. 21st Ann. Int. Conf. Mobile Systems, Applications and Services* 84–95 (ACM, 2023).
24. Chan, J. et al. An off-the-shelf otoacoustic-emission probe for hearing screening via a smartphone. *Nat. Biomed. Eng.* **6**, 1203–1213 (2022).
25. Chan, J. et al. Detecting clinical medication errors with AI enabled wearable cameras. *npj Digit. Med.* **7**, 287 (2024).
26. Palumbo, A. Microsoft HoloLens 2 in medical and healthcare context: state of the art and future prospects. *Sensors* **22**, 7709 (2022).
27. Muensterer, O. J., Lacher, M., Zoeller, C., Bronstein, M. & Kübler, J. Google Glass in pediatric surgery: an exploratory study. *Int. J. Surg.* **12**, 281–289 (2014).
28. Wei, N. J., Dougherty, B., Myers, A. & Badawy, S. M. Using Google Glass in surgical settings: systematic review. *JMIR mHealth uHealth* **6**, e9409 (2018).
29. Chan, J., Rea, T., Gollakota, S. & Sunshine, J. E. Contactless cardiac arrest detection using smart devices. *npj Digit. Med.* **2**, 52 (2019).
30. Song, X. et al. SpiroSonic: monitoring human lung function via acoustic sensing on commodity smartphones. In *Proc. 26th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '20)* 52 (2020).
31. Yin, X. et al. PTEase: objective airway examination for pulmonary telemedicine using commodity smartphones. In *Proc. 21st Ann. Int. Conf. Mobile Systems, Applications and Services* 110–123 (ACM, 2023).
32. Watkins, T. Angelcare recalls baby monitors after 2 deaths. *CNN Health* <https://edition.cnn.com/2013/11/22/health/baby-monitor-recall/> (22 November 2013).
33. Skin integrity issues associated with pulse oximetry. *Pennsylv. PSRS Patient Safety Advis.* **2**, 25–29 (2005).
34. Jin, Y. et al. Earhealth: an earphone-based acoustic otoscope for detection of multiple ear diseases in daily life. In *Proc. 20th Ann. Int. Conf. Mobile Systems, Applications and Services* 397–408 (ACM, 2022).
35. Fan, X., Pearl, D., Howard, R., Shangquan, L. & Thormundsson, T. APG: audioplethysmography for cardiac monitoring in hearables. In *Proc. 29th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '23)* 67 (ACM, 2023).
36. Poets, C. F., Meny, R. G., Chobanian, M. R. & Bonofiglio, R. E. Gasping and other cardiorespiratory patterns during sudden infant deaths. *Pediatr. Res.* **45**, 350–354 (1999).
37. Lumsden, T. Observations on the respiratory centres in the cat. *J. Physiol.* **57**, 153–160 (1923).
38. Zhang, H. et al. PDVocal: towards privacy-preserving Parkinson's disease detection using non-speech body sounds. In *25th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '19)* 16 (ACM, 2019).
39. Rahman, T. et al. BodyBeat: a mobile system for sensing non-speech body sounds. *MobiSys* **14**, 2–594 (2014).
40. Dipinigitis, P. V. Chronic cough due to asthma: ACCP evidence-based clinical practice guidelines. *Chest* **129**, 75S–79S (2006).
41. Fathi, H. et al. Cough in adult cystic fibrosis: diagnosis and response to fundoplication. *Cough* **5**, 1 (2009).
42. Smith, J. & Woodcock, A. Cough and its importance in COPD. *Int. J. Chron. Obstruct. Pulmon. Dis.* **1**, 305–314 (2006).
43. Al Ismail, M., Deshmukh, S. & Singh, R. Detection of COVID-19 through the analysis of vocal fold oscillations. In *Int. Conf. Acoustics, Speech and Signal Processing (ICASSP)* 1035–1039 (IEEE, 2021).
44. Laguarda, J., Hueto, F. & Subirana, B. COVID-19 artificial intelligence diagnosis using only cough recordings. *IEEE Open. J. Eng. Med. Biol.* **1**, 275–281 (2020).
45. Brown, C. et al. Exploring automatic diagnosis of COVID-19 from crowdsourced respiratory sound data. In *Proc. 26th ACM/SIGKDD Int. Conf. Knowledge Discovery and Data Mining* 3474–3484 (ACM, 2020).
46. Pinkas, G. et al. SARS-CoV-2 detection from voice. *IEEE Open. J. Eng. Med. Biol.* **1**, 268–274 (2020).
47. Han, J. et al. Sounds of COVID-19: exploring realistic performance of audio-based digital testing. *npj Digit. Med.* **5**, 16 (2022).
48. Dang, T. et al. Exploring longitudinal cough, breath, and voice data for COVID-19 progression prediction via sequential deep learning: model development and validation. *J. Med. Internet Res.* **24**, e37004 (2022).
49. Whitehill, M., Garrison, J. & Patel, S. Whosecough: in-the-wild cougher verification using multitask learning. In *Int. Conf. Acoustics, Speech and Signal Processing (ICASSP)* 896–900 (IEEE, 2020).
50. Al Hossain, F., Lover, A. A., Corey, G. A., Reich, N. G. & Rahman, T. FluSense: a contactless syndromic surveillance platform for influenza-like illness in hospital waiting areas. *Proc. ACM Interact. Mob. Wearable Ubiquitous Technol.* **4**, 1–28 (2020).
51. Dorafshanian, M., Aitsam, M., Meiri, M. & Di Nuovo, A. Beyond data collection: safeguarding user privacy in social robotics. In *Int. Conf. Industrial Technology (ICIT)* 1–6 (IEEE, 2024).
52. Little, M., McSharry, P., Hunter, E., Spielman, J. & Ramig, L. Suitability of dysphonia measurements for telemonitoring of Parkinson's disease. *IEEE Trans. Biomed. Eng.* **56**, 1015–1022 (2009).
53. Lu, H. et al. Stresssense: detecting stress in unconstrained acoustic environments using smartphones. In *Proc. Conf. Ubiquitous Computing* 351–360 (ACM, 2012).
This article reports a smartphone-based system that detects stress in a user's voice using microphone recordings captured in both indoor and outdoor environments.
54. Rachuri, K. K. et al. EmotionSense: a mobile phones based adaptive platform for experimental social psychology research. In *Proc. 12th Int. Conf. Ubiquitous Computing* 281–290 (ACM, 2010).
This article reports a mobile sensing platform for social psychology studies that uses passive smartphone data to infer individual emotions, activities, and verbal and proximity interactions in a group.
55. Ma, D., Ferlini, A. & Mascolo, C. OESense: employing occlusion effect for in-ear human sensing. In *Proc. 19th Ann. Int. Conf. Mobile Systems, Applications, and Services* 175–187 (ACM, 2021).
56. Butkow, K.-J., Dang, T., Ferlini, A., Ma, D. & Mascolo, C. hEART: motion-resilient heart rate monitoring with in-ear microphones. In *Int. Conf. Pervasive Computing and Communications (PerCom)* 200–209 (IEEE, 2023).
57. Gilliam, F. R. III et al. In-ear infrasonic hemodynamic monitoring with a digital health device for cardiovascular monitoring using the human audiome. *npj Digit. Med.* **5**, 189 (2022).
58. Prakash, J., Yang, Z., Wei, Y.-L., Hassanieh, H. & Choudhury, R. R. EarSense: earphones as a teeth activity sensor. In *Proc. 26th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '20)* 40 (ACM, 2020).
59. Chen, T. et al. Exploring the feasibility of remote cardiac auscultation using earphones. In *Proc. 30th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '24)* 357–372 (ACM, 2024).
60. Larson, E. C. et al. SpiroSmart: using a microphone to measure lung function on a mobile phone. In *Proc. Conf. Ubiquitous Computing* 280–289 (ACM, 2012).
61. Balakrishnan, G., Durand, F. & Gutttag, J. Detecting pulse from head motions in video. In *Proc. IEEE Conf. Computer Vision and Pattern Recognition* 3430–3437 (IEEE, 2013).
62. De Haan, G. & Jeanne, V. Robust pulse rate from chrominance-based rPPG. *IEEE Trans. Biomed. Eng.* **60**, 2878–2886 (2013).
63. Li, X., Chen, J., Zhao, G. & Pietikainen, M. Remote heart rate measurement from face videos under realistic situations. In *Proc. Conf. Computer Vision and Pattern Recognition* 4264–4271 (IEEE, 2014).

64. Poh, M.-Z., McDuff, D. J. & Picard, R. W. Non-contact, automated cardiac pulse measurements using video imaging and blind source separation. *Opt. Express* **18**, 10762–10774 (2010).
65. Poh, M.-Z., McDuff, D. J. & Picard, R. W. Advancements in noncontact, multiparameter physiological measurements using a webcam. *IEEE Trans. Biomed. Eng.* **58**, 7–11 (2010).
66. Tran, D. N., Lee, H. & Kim, C. A robust real time system for remote heart rate measurement via camera. In *Int. Conf. Multimedia and Expo (ICME)* 1–6 (IEEE, 2015).
67. Tulyakov, S. et al. Self-adaptive matrix completion for heart rate estimation from face videos under realistic conditions. In *Proc. Conf. Computer Vision and Pattern Recognition* 2396–2404 (IEEE, 2016).
68. Verkrusye, W., Svaasand, L. O. & Nelson, J. S. Remote plethysmographic imaging using ambient light. *Opt. Express* **16**, 21434–21445 (2008).
69. Adhikary, R., Sadeh, M., Batra, N. & Goel, M. JoulesEye: energy expenditure estimation and respiration sensing from thermal imagery while exercising. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **7**, 1–29 (2024).
70. Mariakakis, A. et al. PupilScreen: using smartphones to assess traumatic brain injury. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **1**, 1–27 (2017).
71. Barry, C. et al. At-home pupillometry using smartphone facial identification cameras. In *Proc. Conf. Human Factors in Computing Systems (CHI '22)* 1–12 (ACM, 2022).
72. Barry, C. & Wang, E. Racially fair pupillometry measurements for RGB smartphone cameras using the far red spectrum. *Sci. Rep.* **13**, 13841 (2023).
73. Mariakakis, A., Wang, E., Patel, S. & Wen, J. C. A smartphone-based system for assessing intraocular pressure. In *38th Ann. Int. Conf. IEEE Engineering in Medicine and Biology Society (EMBC)* 4353–4356 (IEEE, 2016).
74. You, C.-W. et al. Carsafe app: alerting drowsy and distracted drivers using dual cameras on smartphones. In *Proc. 11th Ann. Int. Conf. Mobile Systems, Applications, and Services (MobiSys '13)* 13–26 (ACM, 2013).
75. Khurana, R. & Goel, M. Eyes on the road: detecting phone usage by drivers using on-device cameras. In *Proc. Conf. Human Factors in Computing Systems (CHI '20)* 1–11 (ACM, 2020).
76. Yue, S. & Katabi, D. Liquid testing with your smartphone. In *Proc. 17th Ann. Int. Conf. on Mobile Systems, Applications, and Services (MobiSys '19)* 275–286 (ACM, 2019).
77. Chan, J., Raghunath, A., Michaelsen, K. E. & Gollakota, S. Testing a drop of liquid using smartphone LiDAR. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **6**, 1–27 (2022).
78. Wang, E. J. et al. HemaApp: noninvasive blood screening of hemoglobin using smartphone cameras. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 593–604 (ACM, 2016).
- This article reports a smartphone-based system that noninvasively measures blood haemoglobin concentration by analysing the colour of blood in a user's finger placed over the smartphone camera, using either the built-in light-emitting diode (LED) flash or incandescent light as the illumination source.**
79. Wang, E. J., Zhu, J., Li, W., Rana, R. & Patel, S. HemaApp IR: noninvasive hemoglobin measurement using unmodified smartphone cameras and built-in LEDs. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing and Proc. Int. Symp. Wearable Computers* 305–308 (ACM, 2017).
80. Wang, E. J., Li, W., Zhu, J., Rana, R. & Patel, S. N. Noninvasive hemoglobin measurement using unmodified smartphone camera and white flash. In *39th Ann. Int. Conf. Engineering in Medicine and Biology Society (EMBC)* 2333–2336 (IEEE, 2017).
81. Hoffman, J. S. et al. Smartphone camera oximetry in an induced hypoxemia study. *npj Digit. Med.* **5**, 146 (2022).
82. Bui, N. et al. Pho2: smartphone based blood oxygen level measurement systems using near-IR and red wave-guided light. In *Proc. 15th Conf. Embedded Network Sensor Systems* 26 (ACM, 2017).
83. Wang, E. J. et al. Seismo: blood pressure monitoring using built-in smartphone accelerometer and camera. In *Proc. Conf. Human Factors in Computing Systems (CHI '18)* 425 (ACM, 2018).
84. Xuan, Y. et al. Ultra-low-cost mechanical smartphone attachment for no-calibration blood pressure measurement. *Sci. Rep.* **13**, 8105 (2023).
85. De Greef, L. et al. Bilicam: using mobile phones to monitor newborn jaundice. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 331–342 (ACM, 2014).
- This article reports a smartphone-based system that uses an onboard camera to monitor newborn jaundice by detecting yellow discolouration, and leverages a colour calibration card to ensure consistency across different smartphones.**
86. Taylor, J. A. et al. Use of a smartphone app to assess neonatal jaundice. *Pediatrics* **140**, e20170312 (2017).
87. Mariakakis, A. et al. Biliscreen: smartphone-based scleral jaundice monitoring for liver and pancreatic disorders. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **1**, 1–26 (2017).
88. Mannino, R. G. et al. Smartphone app for non-invasive detection of anemia using only patient-sourced photos. *Nat. Commun.* **9**, 4924 (2018).
89. Babenko, B. et al. Detection of signs of disease in external photographs of the eyes via deep learning. *Nat. Biomed. Eng.* **6**, 1370–1383 (2022).
90. Strutt, J. et al. CAPAPP: smartphone-based capillary refill index assessment in healthy children. In *Proc. Conf. Design of Medical Devices V001T09A009* (ASME, 2023).
91. Eom, S., Sykes, D., Rahimpour, S. & Gorlatova, M. NeuroLens: augmented reality-based contextual guidance through surgical tool tracking in neurosurgery. In *Int. Symp. Mixed and Augmented Reality (ISMAR)* 355–364 (IEEE, 2022).
92. Jin, A. et al. Tool detection and operative skill assessment in surgical videos using region-based convolutional neural networks. In *Winter Conf. Applications of Computer Vision (WACV)* 691–699 (IEEE, 2018).
93. Shi, P., Zhao, Z., Hu, S. & Chang, F. Real-time surgical tool detection in minimally invasive surgery based on attention-guided convolutional neural network. *IEEE Access* **8**, 228853–228862 (2020).
94. Goodman, E. D. et al. Analyzing surgical technique in diverse open surgical videos with multitask machine learning. *JAMA Surg.* **159**, 185–192 (2024).
95. Fujii, R., Saito, H. & Kajita, H. EgoSurgery-tool: a dataset of surgical tool and hand detection from egocentric open surgery videos. Preprint at <https://doi.org/10.48550/arXiv.2406.03095> (2024).
96. Wang, R. et al. Tracking depression dynamics in college students using mobile phone and wearable sensing. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **2**, 43 (2018).
97. Chikersal, P. et al. Detecting depression and predicting its onset using longitudinal symptoms captured by passive sensing: a machine learning approach with robust feature selection. *ACM Trans. Computer-Human Interact. (TOCHI)* **28**, 3 (2021).
98. Huckins, J. F. et al. Mental health and behavior of college students during the early phases of the COVID-19 pandemic: longitudinal smartphone and ecological momentary assessment study. *J. Med. Internet Res.* **22**, e20185 (2020).
99. Wang, R. et al. Predicting symptom trajectories of schizophrenia using mobile sensing. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **1**, 1–24 (2017).
100. Adler, D. A. et al. Predicting early warning signs of psychotic relapse from passive sensing data: an approach using encoder-decoder neural networks. *JMIR mHealth uHealth* **8**, e19962 (2020).
101. Kawsar, F., Min, C., Mathur, A. & Montanari, A. Earables for personal-scale behavior analytics. *IEEE Pervasive Comput.* **17**, 83–89 (2018).
102. Min, C., Mathur, A. & Kawsar, F. Exploring audio and kinetic sensing on earable devices. In *Proc. 4th Worksh. Wearable Systems and Applications* 5–10 (ACM, 2018).
103. Bondareva, E., Hauksdóttir, E. R. & Mascolo, C. Earables for detection of bruxism: a feasibility study. In *Adjunct Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing and Proc. Int. Symp. Wearable Computers* 146–151 (ACM, 2021).
104. Bui, N. et al. eBP: a wearable system for frequent and comfortable blood pressure monitoring from user's ear. In *25th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '19)* 53 (ACM, 2019).
105. Pham, N. et al. WAKE: a behind-the-ear wearable system for microsleep detection. In *Proc. 18th Int. Conf. Mobile Systems, Applications, and Services* 404–418 (ACM, 2020).
106. Nguyen, A. et al. LIBS: a bioelectrical sensing system from human ears for staging whole-night sleep study. *Commun. ACM* **61**, 157–165 (2018).
107. Aziz, A. et al. An unobtrusive and lightweight ear-worn system for continuous epileptic seizure detection. *ACM Trans. Comput. Healthc.* **6**, 6 (2024).
108. Chan, J. et al. PACT: privacy sensitive protocols and mechanisms for mobile contact tracing. *IEEE Data Eng. Bull.* **43**, 15–35 (2020).
109. Stevens, H. & Haines, M. B. TraceTogether: pandemic response, democracy, and technology. *East. Asian Sci. Technol. Soc. Int. J.* **14**, 523–532 (2020).
110. Group, C. P. H. et al. Digital contact tracing technologies in epidemics: a rapid review. *Cochrane Database Syst. Rev.* **8**, CD013699 (2020).
111. Jones, N. R. et al. Two metres or one: what is the evidence for physical distancing in covid-19? *BMJ* **370**, m3223 (2020).
112. Althoff, T. et al. Large-scale physical activity data reveal worldwide activity inequality. *Nature* **547**, 336–339 (2017).
113. Lester, J., Choudhury, T. & Borriello, G. A practical approach to recognizing physical activities. In *4th Int. Conf. Pervasive Computing* 1–16 (ACM, 2006).
114. Lu, H., Pan, W., Lane, N. D., Choudhury, T. & Campbell, A. T. Soundsense: scalable sound sensing for people-centric applications on mobile phones. In *Proc. 7th Int. Conf. Mobile Systems, Applications, and Services* 165–178 (ACM, 2009).
115. Chen, Z. et al. Unobtrusive sleep monitoring using smartphones. In *7th Int. Conf. Pervasive Computing Technologies for Healthcare and Workshops* 145–152 (IEEE, 2013).
116. Lu, H. et al. The jigsaw continuous sensing engine for mobile phone applications. In *Proc. 8th Conf. Embedded Networked Sensor Systems* 71–84 (ACM, 2010).
117. LiKamWa, R., Liu, Y., Lane, N. D. & Zhong, L. Moodscope: building a mood sensor from smartphone usage patterns. In *Proc. 11th Ann. Int. Conf. Mobile Systems, Applications, and Services* 389–402 (ACM, 2013).
118. Lane, N. et al. Bewell: a smartphone application to monitor, model and promote wellbeing. In *5th Int. ICST Conf. Pervasive Computing Technologies for Healthcare* (IEEE, 2012).
119. Lane, N. D. et al. Bewell: sensing sleep, physical activities and social interactions to promote wellbeing. *Mob. Netw. Appl.* **19**, 345–359 (2014).
120. Rabbi, M., Aung, M. H., Zhang, M. & Choudhury, T. MyBehavior: automatic personalized health feedback from user behaviors and preferences using smartphones. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 707–718 (ACM, 2015).
121. Consolvo, S. et al. Activity sensing in the wild: a field trial of UbiFit Garden. In *Proc. SIGCHI Conf. Human Factors in Computing Systems (CHI '08)* 1797–1806 (ACM, 2008).
122. Wang, R., Harari, G., Hao, P., Zhou, X. & Campbell, A. T. SmartGPA: how smartphones can assess and predict academic performance of college students. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 295–306 (ACM, 2015).
123. Ben-Zeev, D., Scherer, E. A., Wang, R., Xie, H. & Campbell, A. T. Next-generation psychiatric assessment: using smartphone sensors to monitor behavior and mental health. *Psychiat. Rehabil. J.* **38**, 218 (2015).

124. Harari, G. M. et al. Using smartphones to collect behavioral data in psychological science: opportunities, practical considerations, and challenges. *Persp. Psychol. Sci.* **11**, 838–854 (2016).
125. Lindhiem, O. et al. Objective measurement of hyperactivity using mobile sensing and machine learning: pilot study. *JMIR Form. Res.* **6**, e35803 (2022).
126. Arakawa, R. et al. Lemurdx: using unconstrained passive sensing for an objective measurement of hyperactivity in children with no parent input. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **7**, 1–23 (2023).
127. Adler, D. A. et al. Identifying mobile sensing indicators of stress-resilience. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **5**, 1–32 (2021).
128. Shao, Q. et al. Joey: supporting kangaroo mother care with computational fabrics. In *Proc. 22nd Ann. Int. Conf. on Mobile Systems, Applications and Services* 237–251 (ACM, 2024).
129. Guo, X. et al. Exploring biomagnetism for inclusive vital sign monitoring: modeling and implementation. In *Proc. 30th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '24)* 93–107 (ACM, 2024).
130. Truong, H. et al. Painometry: wearable and objective quantification system for acute postoperative pain. In *Proc. 18th Int. Conf. Mobile Systems, Applications, and Services* 419–433 (ACM, 2020).
131. Zhou, H. et al. One ring to rule them all: an open source smart ring platform for finger motion analytics and healthcare applications. In *Proc. 8th ACM/IEEE Conf. Internet-of-Things Design and Implementation (IoTDI)* 27–38 (ACM/IEEE, 2023).
132. Zhou, H. et al. SignQuery: a natural user interface and search engine for sign languages with wearable sensors. In *Proc. 29th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '23)* 71 (ACM, 2023).
133. Zhou, H., Lu, T., DeHaan, K. & Gowda, M. ASLRing: American sign language recognition with meta-learning on wearables. In *9th Int. Conf. Internet-of-Things Design and Implementation (IoTDI)* 203–214 (ACM/IEEE, 2024).
134. Yuan, K. et al. ToMoBrush: exploring dental health sensing using a sonic toothbrush. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **8**, 1–27 (2024).
135. Hu, Z., Radmehr, A., Zhang, Y., Pan, S. & Nguyen, P. IOTeeth: intra-oral teeth sensing system for dental occlusal diseases recognition. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **8**, 1–29 (2024).
136. Tasnim Oshim, M. F., Killingback, J., Follette, D., Peng, H. & Rahman, T. MechanoBeat: monitoring interactions with everyday objects using 3D printed harmonic oscillators and ultra-wideband radar. In *Proc. 33rd Ann. Symp. User Interface Software and Technology* 430–444 (ACM, 2020).
137. Iyer, V., Chan, J., Culhane, I., Mankoff, J. & Gollakota, S. Wireless analytics for 3D printed objects. In *Proc. 31st Ann. Symp. User Interface Software and Technology* 141–152 (ACM, 2018).
138. L'heureux, A., Grolinger, K., Elyamany, H. F. & Capretz, M. A. Machine learning with big data: challenges and approaches. *IEEE Access* **5**, 7776–7797 (2017).
139. Baltrušaitis, T., Ahuja, C. & Morency, L.-P. Multimodal machine learning: a survey and taxonomy. *IEEE Trans. Pattern Anal. Mach. Intell.* **41**, 423–443 (2018).
140. Rai, A., Chintalapudi, K. K., Padmanabhan, V. N. & Sen, R. Zee: zero-effort crowdsourcing for indoor localization. In *Proc. 18th Ann. Int. Conf. Mobile Computing and Networking (MobiCom '12)* 293–304 (ACM, 2012).
141. Brajdic, A. & Harle, R. Walk detection and step counting on unconstrained smartphones. In *Proc. Int. Joint Conf. Pervasive and Ubiquitous Computing* 225–234 (ACM, 2013).
142. Seyyed-Kalantari, L., Zhang, H., McDermott, M. B., Chen, I. Y. & Ghassemi, M. Underdiagnosis bias of artificial intelligence algorithms applied to chest radiographs in under-served patient populations. *Nat. Med.* **27**, 2176–2182 (2021).
143. Burlina, P., Joshi, N., Paul, W., Pacheco, K. D. & Bressler, N. M. Addressing artificial intelligence bias in retinal diagnostics. *Transl. Vis. Sci. Technol.* **10**, 13 (2021).
144. Gianattasio, K. Z., Ciarleglio, A. & Power, M. C. Development of algorithmic dementia ascertainment for racial/ethnic disparities research in the US health and retirement study. *Epidemiology* **31**, 126–133 (2020).
145. Park, Y. et al. Comparison of methods to reduce bias from clinical prediction models of postpartum depression. *JAMA Netw. Open* **4**, e213909 (2021).
146. van Breugel, B., Liu, T., Oglic, D. & van der Schaar, M. Synthetic data in biomedicine via generative artificial intelligence. *Nat. Rev. Bioeng.* **2**, 991–1004 (2024).
147. Goodfellow, I. et al. Generative adversarial networks. *Commun. ACM* **63**, 139–144 (2020).
148. Kingma, D. P. & Welling, M. Auto-encoding variational Bayes. Preprint at <https://doi.org/10.48550/arXiv.1312.6114> (2013).
149. Arora, A. & Arora, A. Generative adversarial networks and synthetic patient data: current challenges and future perspectives. *Future Healthc. J.* **9**, 190 (2022).
150. Wan, Z., Zhang, Y. & He, H. Variational autoencoder based synthetic data generation for imbalanced learning. In *Symp. Series Computational Intelligence (SSCI)* 1–7 (IEEE, 2017).
151. Li, Z., Zhu, H., Lu, Z. & Yin, M. Synthetic data generation with large language models for text classification: potential and limitations. In *Proc. 2023 Conf. Empirical Methods in Natural Language Processing (ACL)*, 2023).
152. Viceconti, M. et al. In silico trials: verification, validation and uncertainty quantification of predictive models used in the regulatory evaluation of biomedical products. *Methods* **185**, 120–127 (2021).
153. Lecomte, F., Alvarez, P., Cotin, S. & Dillenseger, J.-L. Beyond respiratory models: a physics-enhanced synthetic data generation method for 2D–3D deformable registration. In *Proc. IEEE/CVF Conf. Computer Vision and Pattern Recognition* 2413–2421 (IEEE, 2024).
154. Myles, P., Ordish, J. & Tucker, A. The potential synergies between synthetic data and in silico trials in relation to generating representative virtual population cohorts. *Prog. Biomed. Eng.* **5**, 013001 (2023).
155. Moss, A. J. Gender differences in ECG parameters and their clinical implications. *Ann. Noninvasive Electrocardiol.* **15**, 1–2 (2010).
156. Khane, R. S. & Surdi, A. D. Gender differences in the prevalence of electrocardiogram abnormalities in the elderly: a population survey in India. *Iran. J. Med. Sci.* **37**, 92–99 (2012).
157. Nigg, B., Fisher, V. & Ronsky, J. Gait characteristics as a function of age and gender. *Gait Posture* **2**, 213–220 (1994).
158. McKean, K. A. et al. Gender differences exist in osteoarthritic gait. *Clin. Biomech.* **22**, 400–409 (2007).
159. Yu, S., Tan, T., Huang, K., Jia, K. & Wu, X. A study on gait-based gender classification. *IEEE Trans. Image Process.* **18**, 1905–1910 (2009).
160. Allen, J. & Murray, A. Age-related changes in the characteristics of the photoplethysmographic pulse shape at various body sites. *Physiol. Meas.* **24**, 297–307 (2003).
161. Yousef, Q., Reaz, M. & Ali, M. A. M. The analysis of PPG morphology: investigating the effects of aging on arterial compliance. *Meas. Sci. Rev.* **12**, 266–271 (2012).
162. Fouzas, S., Pifitis, K. N. & Anthracopoulos, M. B. Pulse oximetry in pediatric practice. *Pediatrics* **128**, 740–752 (2011).
163. Picone, D. S. et al. Influence of age on upper arm cuff blood pressure measurement. *Hypertension* **75**, 844–850 (2020).
164. Feiner, J. R., Severinghaus, J. W. & Bickler, P. E. Dark skin decreases the accuracy of pulse oximeters at low oxygen saturation: the effects of oximeter probe type and gender. *Anesth. Analg.* **105**, S18–S23 (2007).
165. Colvonen, P. J. Response to: investigating sources of inaccuracy in wearable optical heart rate sensors. *npj Digit. Med.* **4**, 38 (2021).
166. Keller, M. D., Harrison-Smith, B., Patil, C. & Arefin, M. S. Skin colour affects the accuracy of medical oxygen sensors. *Nature* **610**, 449–451 (2022).
167. Henry, N. R. et al. Disparities in hypoxemia detection by pulse oximetry across self-identified racial groups and associations with clinical outcomes. *Crit. Care Med.* **50**, 204–211 (2022).
168. Schlosman, D. & Elliott, M. Sleep.3: clinical presentation and diagnosis of the obstructive sleep apnoea hypopnoea syndrome. *Thorax* **59**, 347–352 (2004).
169. Benzeghiba, M. et al. Automatic speech recognition and speech variability: a review. *Speech Commun.* **49**, 763–786 (2007).
170. Koenecke, A. et al. Racial disparities in automated speech recognition. *Proc. Natl Acad. Sci. USA* **117**, 7684–7689 (2020).
171. Hwang, W.-C., Myers, H. F., Abe-Kim, J. & Ting, J. Y. A conceptual paradigm for understanding culture's impact on mental health: the cultural influences on mental health (CIMH) model. *Clin. Psychol. Rev.* **28**, 211–227 (2008).
172. Henry, C. J., Quek, R. Y. C., Kaur, B., Shyam, S. & Singh, H. K. G. A glycaemic index compendium of non-Western foods. *Nutr. Diabetes* **11**, 2 (2021).
173. Owen, M. et al. Diversity, equity, and inclusion in I&M: beyond the technology: wearables and the cultural compass. *IEEE Instrum. Meas. Mag.* **27**, 38–43 (2024).
174. Pereira, T. et al. Photoplethysmography based atrial fibrillation detection: a review. *npj Digit. Med.* **3**, 3 (2020).
175. Niemelä, M. J., Airaksinen, K. J. & Huikuri, H. V. Effect of beta-blockade on heart rate variability in patients with coronary artery disease. *J. Am. Coll. Cardiol.* **23**, 1370–1377 (1994).
176. Eichellbaum, M. Drug metabolism in thyroid disease. *Clin. Pharmacokinet.* **1**, 339–350 (1976).
177. van Zyl, L. T., Hasegawa, T. & Nagata, K. Effects of antidepressant treatment on heart rate variability in major depression: a quantitative review. *Biopsychosoc. Med.* **2**, 12 (2008).
178. Wichniak, A., Wierzbicka, A., Walęcka, M. & Jernajczyk, W. Effects of antidepressants on sleep. *Curr. Psychiatry Rep.* **19**, 1–7 (2017).
179. Wang, X. & Luan, W. Research progress on digital health literacy of older adults: a scoping review. *Front. Public Health* **10**, 906089 (2022).
180. Kemp, E. et al. Health literacy, digital health literacy and the implementation of digital health technologies in cancer care: the need for a strategic approach. *Health Promot. J. Austr.* **32**, 104–114 (2021).
181. Tegegne, M. D. et al. Digital literacy level and associated factors among health professionals in a referral and teaching hospital: an implication for future digital health systems implementation. *Front. Public Health* **11**, 1130894 (2023).
182. Adjekum, A., Blasimme, A. & Vayena, E. Elements of trust in digital health systems: scoping review. *J. Med. Internet Res.* **20**, e11254 (2018).
183. Blalock, D., Gonzalez Ortiz, J. J., Frankle, J. & Gutttag, J. What is the state of neural network pruning? *Proc. Mach. Learn. Syst.* **2**, 129–146 (2020).
184. Guo, Y. A survey on methods and theories of quantized neural networks. Preprint at <https://doi.org/10.48550/arXiv.1808.04752> (2018).
185. Gou, J., Yu, B., Maybank, S. J. & Tao, D. Knowledge distillation: a survey. *Int. J. Comput. Vis.* **129**, 1789–1819 (2021).
186. Bucilua, C., Caruana, R. & Niculescu-Mizil, A. Model compression. In *Proc. 12th ACM/SIGKDD Int. Conf. Knowledge Discovery and Data Mining* 535–541 (ACM, 2006).
187. Sainath, T. N., Kingsbury, B., Sindhwani, V., Arisoy, E. & Ramabhadran, B. Low-rank matrix factorization for deep neural network training with high-dimensional output targets. In *Int. Conf. Acoustics, Speech and Signal Processing (ICASSP)* 6655–6659 (IEEE, 2013).

188. Elsken, T., Metzner, J. H. & Hutter, F. Neural architecture search: a survey. *J. Mach. Learn. Res.* **20**, 1–21 (2019).
189. Nguyen, D. C. et al. Federated learning for smart healthcare: a survey. *ACM Comput. Surv. (CSUR)* **55**, 60 (2022).
190. Xu, J. et al. Federated learning for healthcare informatics. *J. Healthc. Inform. Res.* **5**, 1–19 (2021).
191. Choudhury, O. et al. Anonymizing data for privacy-preserving federated learning. In *ECAI 2020, 24th European Conference on Artificial Intelligence* (IOS Press, 2020).
192. Iravantchi, Y., Ahuja, K., Goel, M., Harrison, C. & Sample, A. PrivacyMic: utilizing inaudible frequencies for privacy preserving daily activity recognition. In *Proc. Conf. Human Factors in Computing Systems (CHI '21)* 198 (ACM, 2021).
193. Acar, A., Aksu, H., Uluagac, A. S. & Conti, M. A survey on homomorphic encryption schemes: theory and implementation. *ACM Comput. Surv. (CSUR)* **51**, 79 (2018).
194. Sagi, D., Spitzer-Shohat, S., Schuster, M., Daudi, L. & Rudolf, M. C. J. Teaching plain language to medical students: improving communication with disadvantaged patients. *BMC Med. Educ.* **21**, 407 (2021).
195. Pinaya, W. H. et al. Brain imaging generation with latent diffusion models. In *MICCAI Worksh. Deep Generative Models* 117–126 (Springer, 2022).
196. Simonyan, K., Vedaldi, A. & Zisserman, A. Deep inside convolutional networks: visualising image classification models and saliency maps. In *Workshop at International Conference on Learning Representations (ICLR, 2013)*.
197. Kim, B. et al. Interpretability beyond feature attribution: quantitative testing with concept activation vectors (TCAV). In *Int. Conf. Machine Learning* 2668–2677 (PMLR, 2018).
198. Krause, J. et al. Grader variability and the importance of reference standards for evaluating machine learning models for diabetic retinopathy. *Ophthalmology* **125**, 1264–1272 (2018).
199. Lundberg, S. M. & Lee, S.-I. A unified approach to interpreting model predictions. In *Proc. 31st Int. Conf. Neural Information Processing Systems (NIPS '17)* 4768–4777 (ACM, 2017).
200. Lundberg, S. M. et al. Explainable machine-learning predictions for the prevention of hypoxaemia during surgery. *Nat. Biomed. Eng.* **2**, 749–760 (2018).
201. Ribeiro, M. T., Singh, S. & Guestrin, C. 'Why should I trust you?' Explaining the predictions of any classifier. In *Proc. 22nd ACM/SIGKDD Int. Conf. Knowledge Discovery and Data Mining* 1135–1144 (ACM, 2016).
202. Lechner, N. H. An overview of cybersecurity regulations and standards for medical device software. In *Central Eur. Conf. Information and Intelligent Systems* 237–249 (Faculty of Organization and Informatics, 2017).
203. Schmidt, A. Regulatory challenges in healthcare IT: ensuring compliance with HIPAA and GDPR. *Acad. J. Sci. Technol.* **3**, 1–7 (2020).
204. Cohen, I. G., Gerke, S. & Kramer, D. B. Ethical and legal implications of remote monitoring of medical devices. *Milbank Q.* **98**, 1257–1289 (2020).
205. Alzghabi, H. Examining healthcare practitioners' perceptions of virtual physicians, mHealth applications, and barriers to adoption: insights for improving patient care and digital health integration. *Int. J. Gen. Med.* **18**, 1865–1885 (2025).
206. Guo, X., Zhang, X. & Sun, Y. The privacy–personalization paradox in mHealth services acceptance of different age groups. *Electron. Commer. Res. Appl.* **16**, 55–65 (2016).
207. Koelle, M., Wolf, K. & Boll, S. Beyond LED status lights–design requirements of privacy notices for body-worn cameras. In *Proc. 12th Int. Conf. on Tangible, Embedded, and Embodied Interaction* 177–187 (ACM, 2018).
208. Lindgren, D., Karegar, F., Kane, B. & Pettersson, J. S. An evaluation of three designs to engage users when providing their consent on smartphones. *Behav. Inf. Technol.* **40**, 398–414 (2021).
209. Ayaz, M., Pasha, M. F., Alzahrani, M. Y., Budiarto, R. & Stiawan, D. The fast health interoperability resources (FHIR) standard: systematic literature review of implementations, applications, challenges and opportunities. *JMIR Med. Inform.* **9**, e21929 (2021).
210. Dotson, P. CPT® codes: what are they, why are they necessary, and how are they developed? *Adv. Wound Care* **2**, 583–587 (2013).
211. Chan, J. et al. Closed-loop wearable naloxone injector system. *Sci. Rep.* **11**, 22663 (2021).
212. Mitrasinovic, S. et al. Clinical and surgical applications of smart glasses. *Technol. Health Care* **23**, 381–401 (2015).
213. Breda, J., Springston, M., Mariakakis, A. & Patel, S. Feverphone: accessible core-body temperature sensing for fever monitoring using commodity smartphones. *Proc. ACM Interact. Mob. Wearable Ubiqu. Technol.* **7**, 1–23 (2023).
214. Preston, J., Brown, F. W. & Hartley, B. Using telemedicine to improve health care in distant areas. *Psychiat. Serv.* **43**, 25–32 (1992).
215. Anawade, P. A., Sharma, D. & Gahane, S. A comprehensive review on exploring the impact of telemedicine on healthcare accessibility. *Cureus* **16**, e55996 (2024).
216. Vesga, O. et al. Highly sensitive scent-detection of COVID-19 patients in vivo by trained dogs. *PLoS ONE* **16**, e0257474 (2021).
217. Rooney, N. J., Morant, S. & Guest, C. Investigation into the value of trained glycaemia alert dogs to clients with type 1 diabetes. *PLoS ONE* **8**, e69921 (2013).
218. Cornu, J.-N., Cancel-Tassin, G., Ondet, V., Girardet, C. & Cussenot, O. Olfactory detection of prostate cancer by dogs sniffing urine: a step forward in early diagnosis. *Eur. Urol.* **59**, 197–201 (2011).
219. Willis, C. M. et al. Olfactory detection of human bladder cancer by dogs: proof of principle study. *BMJ* **329**, 712 (2004).
220. Strauch, M. et al. More than apples and oranges — detecting cancer with a fruit fly's antenna. *Sci. Rep.* **4**, 3576 (2014).
221. Qin, C. et al. Artificial olfactory biohybrid system: an evolving sense of smell. *Adv. Sci.* **10**, 2204726 (2023).
222. Sakar, B. E. et al. Collection and analysis of a Parkinson speech dataset with multiple types of sound recordings. *IEEE J. Biomed. Health Inform.* **17**, 828–834 (2013).

Author contributions

J.C., R.N. and S.G. researched data for the manuscript and contributed to discussion of its contents. J.C. and R.N. wrote the article. M.G. reviewed the manuscript. All authors edited the manuscript.

Competing interests

The authors declare the following competing interests: S.G. and J.C. are co-founders of Wavely Diagnostics, Inc. The remaining authors declare no competing interests.

Citation diversity statement

We acknowledge that papers authored by scholars from historically excluded groups are systematically under-cited. Here, we have made every attempt to reference relevant papers in a manner that is equitable in terms of racial, ethnic, gender and geographical representation.

Additional information

Peer review information *Nature Reviews Bioengineering* thanks Ting Dang, Noe Brasier and the other, anonymous, reviewer(s) for their contribution to the peer review of this work.

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Springer Nature or its licensor (e.g. a society or other partner) holds exclusive rights to this article under a publishing agreement with the author(s) or other rightsholder(s); author self-archiving of the accepted manuscript version of this article is solely governed by the terms of such publishing agreement and applicable law.

Related links

Action plan: <https://www.fda.gov/medical-devices/software-medical-device-samd/artificial-intelligence-and-machine-learning-software-medical-device>

Active sonar technology for smartphones: https://www.accessdata.fda.gov/cdrh_docs/pdf21/K211387.pdf

Android API: <https://developer.android.com/guide/practices/compatibility>

Blood oxygen: <https://support.ouraring.com/hc/en-us/articles/7328398760851-Blood-Oxygen-Sensing-SpO2>

Blood pressure: <https://www.samsung.com/ae/support/apps-services/how-to-measure-blood-pressure-using-a-galaxy-watch/>

Body composition: <https://www.samsung.com/uk/support/mobile-devices/measure-your-body-composition-with-the-galaxy-watch-series/>

BreatheEasy: https://www.accessdata.fda.gov/cdrh_docs/pdf21/K211387.pdf

Capture breathing rate by tracking chest movements from the front-facing camera:

<https://blog.google/technology/health/take-pulse-health-and-wellness-your-phone/>

Car crash detection: <https://store.google.com/intl/en/ideas/articles/car-crash-detection/>

Coarse-grained location estimates: <https://maps.google.com/how-accurate-is-gps/>

Digital Wellbeing app: <https://blog.google/products/pixel/health-ai-better-sleep/>

ECG app: <https://support.apple.com/en-us/120278>

Exposure notifications: <https://about.google/company-info/commitments/>

Fall detection: <https://support.apple.com/en-us/108896>

FDA has approved mobile medical systems that leverage device sensors: <https://web.archive.org/web/20220308170430/https://www.fda.gov/medical-devices/device-software-functions-including-mobile-medical-applications/examples-premarket-submissions-include-mmars-cleared-or-approved-fda>

FDA-granted smartphone app for body-temperature monitoring: <https://blog.google/products/pixel/google-thermometer-app-body-temperature/>

Google Fit app for Pixel phones: <https://blog.google/technology/health/take-pulse-health-and-wellness-your-phone/>

Guidance for mobile medical applications: <https://www.fda.gov/regulatory-information/search-fda-guidance-documents/policy-device-software-functions-and-mobile-medical-applications>

Hear the World: <https://www.hear-the-world.com/>

Hearing-screening devices: <https://www.e3diagnostics.com/products/otoacoustic-emissions---oe/grason-stadler-corti>

Heart rate: <https://support.ouraring.com/hc/en-us/articles/4410656562579-Heart-Rate-Graph>

Irregular heart rhythm: <https://support.apple.com/en-us/120276>

Irregular heart rhythms: https://store.google.com/magazine/fitbit_irregular_rhythm?pli=1&hl=en-US

Loss of pulse detection: <https://blog.google/feed/pixel-watch-3-loss-of-pulse-detection-fda/>

Measure colour changes caused by blood moving through the fingertip to compute heart rate: <https://blog.google/technology/health/take-pulse-health-and-wellness-your-phone/>

Medical device academy: <https://medicaldeviceacademy.com/510k-cost/>

Minuteful Kidney: <https://blog.healthy.io/company-news/minuteful-kidney-receives-fda-clearance/>

Mobile medical apps: <https://web.archive.org/web/20220308170430/https://www.fda.gov/medical-devices/device-software-functions-including-mobile-medical-applications/examples-premarket-submissions-include-mmms-cleared-or-approved-fda>

NOVID: <https://www.novid.org/>

Predict the start of the menstrual period: <https://ouraring.com/womens-health>

SENSORA digital stethoscope: <https://www.ekohealth.com/blogs/newsroom/eko-announces-new-category-iii-cpt-code>

Sleep sensing algorithms: <https://blog.google/products/google-nest/new-nest-hub-soli/>

SleepScore app: <https://apps.apple.com/us/app/sleepscore/id1364781299>

Software as a medical device: <https://www.fda.gov/medical-devices/software-medical-device-samd/what-are-examples-software-medical-device>

Sonar-based breathing monitors: <https://www.mobihealthnews.com/news/sound-life-sciences-scores-fda-510k-smart-device-respiratory-monitoring-app>

The SleepScore app: <https://apps.apple.com/us/app/sleepscore/id1364781299>

TraceTogether: <https://github.com/opentrace-community/opentrace-calibration/blob/master/Trial%20Methodologies.md>

Wristbands: <https://www.empatica.com/embrace2/>

© Springer Nature Limited 2025